

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037704.D
 Acq On : 01 Oct 2024 15:39
 Operator : SY/MD
 Sample : P4206-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	324697	356543	15.10%	2.074%
2	1.532	146	153	170	rVB	276723	331985	14.06%	1.931%
3	2.059	308	317	333	rBV	569592	817802	34.64%	4.758%
4	3.490	758	762	764	rBV3	646	462	0.02%	0.003%
5	3.735	836	838	840	rBV3	471	243	0.01%	0.001%
6	3.796	849	857	892	rBV	101291	282548	11.97%	1.644%
7	4.243	980	996	1025	rBV	379442	972539	41.19%	5.658%
8	4.577	1096	1100	1101	rBV2	550	410	0.02%	0.002%
9	4.638	1114	1119	1123	rBV4	979	859	0.04%	0.005%
10	4.657	1123	1125	1127	rVV2	889	398	0.02%	0.002%
11	4.674	1127	1130	1132	rVB2	587	370	0.02%	0.002%
12	4.712	1140	1142	1145	rBV4	384	245	0.01%	0.001%
13	4.728	1145	1147	1149	rBV2	706	333	0.01%	0.002%
14	4.796	1164	1168	1169	rBV2	422	294	0.01%	0.002%
15	4.809	1169	1172	1173	rVV2	436	237	0.01%	0.001%
16	4.844	1177	1183	1186	rBV3	674	647	0.03%	0.004%
17	4.883	1191	1195	1196	rBV2	345	204	0.01%	0.001%
18	4.950	1200	1216	1251	rBV2	930339	2360920	100.00%	13.736%
19	5.452	1368	1372	1374	rBV4	481	367	0.02%	0.002%
20	5.465	1374	1376	1377	rBV	670	356	0.02%	0.002%
21	5.529	1385	1396	1430	rBV	690755	1434450	60.76%	8.346%
22	5.985	1522	1538	1564	rBV	523444	1086533	46.02%	6.321%
23	6.445	1679	1681	1685	rVB2	719	379	0.02%	0.002%
24	6.468	1685	1688	1689	rBV	518	205	0.01%	0.001%
25	6.497	1695	1697	1700	rBV3	566	319	0.01%	0.002%
26	6.519	1703	1704	1707	rBV2	603	286	0.01%	0.002%
27	6.535	1707	1709	1710	rBV	450	212	0.01%	0.001%
28	6.567	1717	1719	1721	rBV2	540	300	0.01%	0.002%
29	6.664	1747	1749	1752	rVB2	492	178	0.01%	0.001%
30	6.702	1757	1761	1764	rBV4	662	484	0.02%	0.003%
31	6.735	1769	1771	1773	rBV	740	386	0.02%	0.002%
32	6.831	1797	1801	1803	rBV4	397	232	0.01%	0.001%
33	6.844	1803	1805	1808	rBV2	485	305	0.01%	0.002%
34	6.866	1810	1812	1814	rBV2	569	247	0.01%	0.001%
35	6.911	1815	1826	1857	rBV	262782	520478	22.05%	3.028%
36	7.239	1917	1928	1970	rBV	1035048	1860657	78.81%	10.825%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037704.D
 Acq On : 01 Oct 2024 15:39
 Operator : SY/MD
 Sample : P4206-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2055	rBV	179364	339117	14.36%	1.973%
38	7.995	2160	2163	2164	rBV2	795	481	0.02%	0.003%
39	8.024	2164	2172	2212	rVV	303875	666878	28.25%	3.880%
40	8.509	2320	2323	2327	rBV4	1321	979	0.04%	0.006%
41	8.622	2356	2358	2364	rBV5	1126	1189	0.05%	0.007%
42	8.779	2396	2407	2436	rBV	1072507	1791307	75.87%	10.422%
43	9.197	2535	2537	2541	rVB3	1090	653	0.03%	0.004%
44	9.259	2552	2556	2557	rBV4	656	484	0.02%	0.003%
45	9.297	2566	2568	2570	rBV2	762	472	0.02%	0.003%
46	9.352	2583	2585	2587	rBV2	364	176	0.01%	0.001%
47	9.458	2615	2618	2621	rBV4	786	703	0.03%	0.004%
48	9.545	2642	2645	2647	rBV2	553	324	0.01%	0.002%
49	9.564	2647	2651	2653	rBV3	769	539	0.02%	0.003%
50	9.603	2660	2663	2664	rBV2	662	446	0.02%	0.003%
51	9.638	2671	2674	2677	rBV3	453	309	0.01%	0.002%
52	9.699	2690	2693	2696	rBV3	717	565	0.02%	0.003%
53	9.718	2696	2699	2704	rVV6	1011	1043	0.04%	0.006%
54	9.757	2708	2711	2714	rVB3	900	439	0.02%	0.003%
55	9.773	2714	2716	2720	rBV4	479	310	0.01%	0.002%
56	9.831	2732	2734	2737	rBV3	426	205	0.01%	0.001%
57	9.966	2770	2776	2779	rVB4	861	811	0.03%	0.005%
58	9.988	2779	2783	2785	rBV3	707	592	0.03%	0.003%
59	10.043	2798	2800	2803	rBV2	561	330	0.01%	0.002%
60	10.069	2805	2808	2810	rVB4	887	514	0.02%	0.003%
61	10.146	2820	2832	2856	rBV	610829	964322	40.85%	5.610%
62	10.304	2877	2881	2884	rBV5	1232	1168	0.05%	0.007%
63	10.423	2917	2918	2920	rBV2	430	148	0.01%	0.001%
64	10.445	2923	2925	2927	rVV3	467	133	0.01%	0.001%
65	10.654	2987	2990	2991	rBV2	533	294	0.01%	0.002%
66	10.686	2998	3000	3004	rVB4	1102	611	0.03%	0.004%
67	10.718	3004	3010	3014	rBV6	898	1114	0.05%	0.006%
68	10.776	3025	3028	3032	rBV3	1302	1333	0.06%	0.008%
69	10.837	3046	3047	3050	rVB	643	247	0.01%	0.001%
70	10.866	3053	3056	3059	rBV2	618	447	0.02%	0.003%
71	10.931	3074	3076	3078	rBV2	415	210	0.01%	0.001%
72	10.985	3091	3093	3094	rBV	489	257	0.01%	0.001%
73	11.123	3132	3136	3140	rBV6	1386	1446	0.06%	0.008%
74	11.178	3142	3153	3189	rVV	1042403	1680259	71.17%	9.776%
75	11.490	3246	3250	3253	rBV4	910	722	0.03%	0.004%
76	11.554	3258	3270	3301	rVV	1037939	1690612	71.61%	9.836%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037704.D
Acq On : 01 Oct 2024 15:39
Operator : SY/MD
Sample : P4206-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	12.557	3578	3582	3584	rBV4	703	589	0.02%	0.003%
78	12.747	3639	3641	3642	rBV2	682	272	0.01%	0.002%
79	12.879	3679	3682	3685	rBV2	856	641	0.03%	0.004%
80	13.323	3817	3820	3823	rBV2	892	748	0.03%	0.004%
81	13.921	4004	4006	4008	rBV3	565	317	0.01%	0.002%

Sum of corrected areas: 17188169




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037704.D
Acq On : 01 Oct 2024 15:39
Operator : SY/MD
Sample : P4206-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

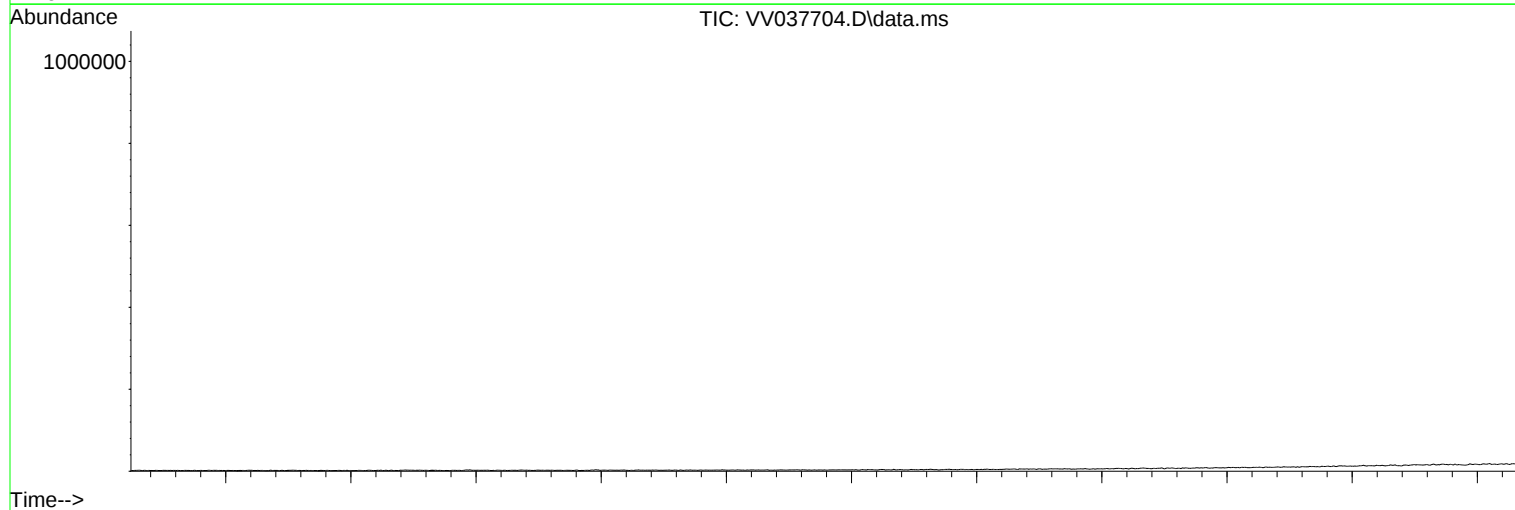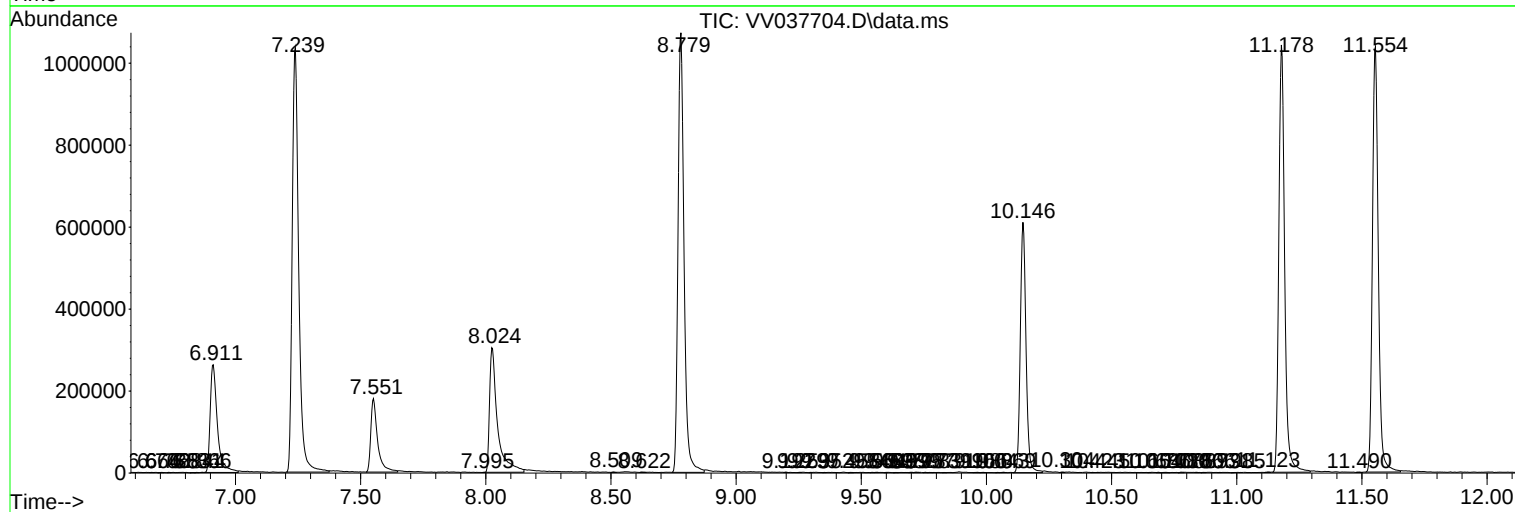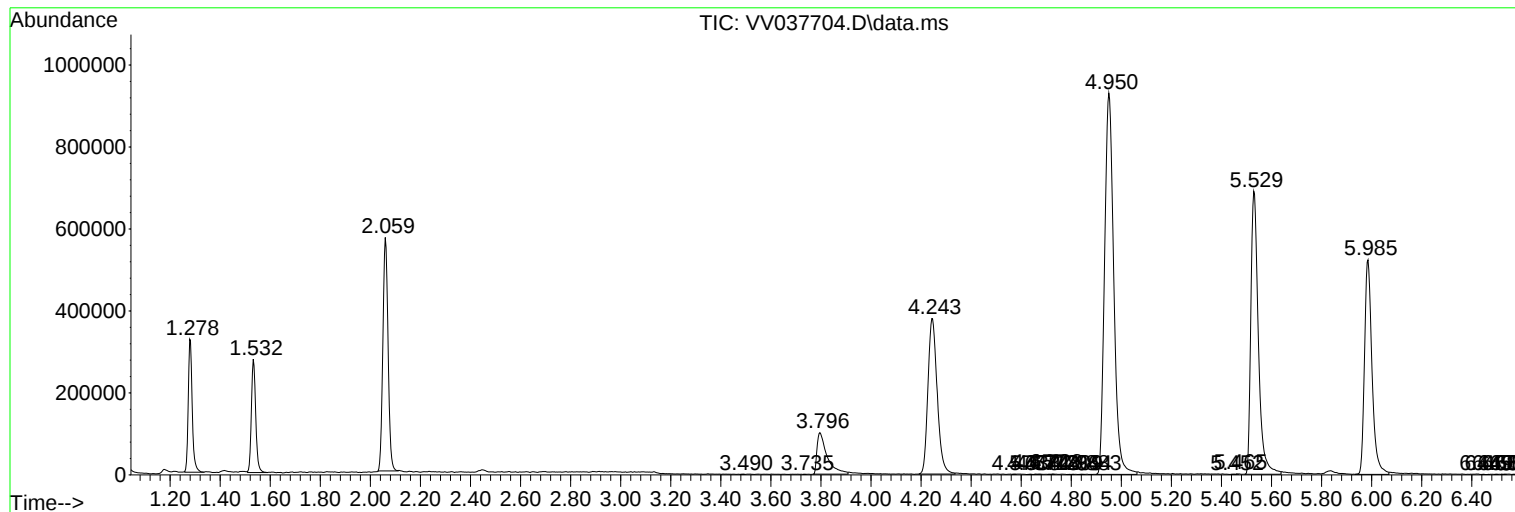

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037704.D
Acq On : 01 Oct 2024 15:39
Operator : SY/MD
Sample : P4206-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037704.D
Acq On : 01 Oct 2024 15:39
Operator : SY/MD
Sample : P4206-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------