

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037705.D
 Acq On : 01 Oct 2024 16:00
 Operator : SY/MD
 Sample : P4203-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.178	37	43	51	rBV	10294	17094	0.71%	0.097%
2	1.281	68	75	89	rBV	335003	360318	14.98%	2.053%
3	1.532	146	153	165	rVB	280053	330375	13.73%	1.883%
4	2.059	308	317	333	rVB	582703	833662	34.65%	4.751%
5	3.336	712	714	716	rBV	681	394	0.02%	0.002%
6	3.461	751	753	758	rVB2	442	307	0.01%	0.002%
7	3.535	773	776	777	rBV2	553	265	0.01%	0.002%
8	3.548	778	780	782	rVV2	578	241	0.01%	0.001%
9	3.577	786	789	792	rBV3	741	541	0.02%	0.003%
10	3.683	820	822	825	rVB3	505	232	0.01%	0.001%
11	3.796	848	857	890	rBV	102714	292782	12.17%	1.668%
12	4.243	982	996	1026	rVB	388222	983274	40.87%	5.603%
13	4.645	1115	1121	1123	rBV3	726	654	0.03%	0.004%
14	4.670	1127	1129	1131	rVB2	655	258	0.01%	0.001%
15	4.728	1145	1147	1150	rVB3	729	310	0.01%	0.002%
16	4.747	1150	1153	1154	rBV2	588	307	0.01%	0.002%
17	4.780	1162	1163	1164	rBV	298	108	0.00%	0.001%
18	4.950	1199	1216	1248	rBV2	949339	2406120	100.00%	13.712%
19	5.529	1385	1396	1426	rBV	701425	1462650	60.79%	8.335%
20	5.985	1526	1538	1568	rBV	524130	1101831	45.79%	6.279%
21	6.349	1645	1651	1652	rBV4	718	696	0.03%	0.004%
22	6.487	1692	1694	1696	rBV3	436	138	0.01%	0.001%
23	6.500	1696	1698	1701	rVV	453	294	0.01%	0.002%
24	6.673	1749	1752	1755	rBV2	726	453	0.02%	0.003%
25	6.718	1763	1766	1767	rBV2	781	364	0.02%	0.002%
26	6.776	1781	1784	1785	rBV2	646	251	0.01%	0.001%
27	6.818	1794	1797	1798	rBV2	663	376	0.02%	0.002%
28	6.870	1810	1813	1814	rBV2	452	268	0.01%	0.002%
29	6.908	1814	1825	1859	rVV	269891	531873	22.11%	3.031%
30	7.239	1917	1928	1962	rBV	1061123	1897558	78.86%	10.814%
31	7.551	2016	2025	2054	rBV	180561	349231	14.51%	1.990%
32	7.956	2148	2151	2155	rVB3	1288	724	0.03%	0.004%
33	7.989	2160	2161	2163	rVB3	983	287	0.01%	0.002%
34	8.024	2163	2172	2219	rBV	313072	707667	29.41%	4.033%
35	8.693	2377	2380	2386	rBV4	1010	924	0.04%	0.005%
36	8.728	2389	2391	2393	rVB2	658	254	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037705.D
 Acq On : 01 Oct 2024 16:00
 Operator : SY/MD
 Sample : P4203-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.779	2396	2407	2435	rBV	1105645	1835023	76.26%	10.457%
38	9.294	2565	2567	2571	rVB2	945	676	0.03%	0.004%
39	9.358	2584	2587	2589	rVB3	1041	599	0.02%	0.003%
40	9.381	2589	2594	2596	rBV4	1291	1091	0.05%	0.006%
41	9.451	2611	2616	2617	rBV3	555	465	0.02%	0.003%
42	9.542	2641	2644	2646	rVB2	853	486	0.02%	0.003%
43	9.554	2646	2648	2651	rBV2	428	295	0.01%	0.002%
44	9.570	2651	2653	2657	rBV	644	465	0.02%	0.003%
45	9.622	2666	2669	2673	rVB3	830	608	0.03%	0.003%
46	9.641	2673	2675	2678	rBV2	789	324	0.01%	0.002%
47	9.677	2682	2686	2687	rBV2	777	560	0.02%	0.003%
48	9.808	2723	2727	2730	rVB3	883	522	0.02%	0.003%
49	9.831	2730	2734	2737	rBV4	1066	979	0.04%	0.006%
50	9.927	2761	2764	2765	rBV2	683	375	0.02%	0.002%
51	9.947	2768	2770	2778	rVB4	859	750	0.03%	0.004%
52	10.024	2787	2794	2797	rBV5	771	1008	0.04%	0.006%
53	10.146	2821	2832	2858	rBV	617517	983630	40.88%	5.605%
54	10.490	2937	2939	2942	rBV2	683	326	0.01%	0.002%
55	10.509	2942	2945	2948	rBV2	563	384	0.02%	0.002%
56	10.529	2948	2951	2953	rBV3	1094	616	0.03%	0.004%
57	10.590	2967	2970	2972	rBV3	157	71	0.00%	0.000%
58	10.599	2972	2973	2976	rVB	536	239	0.01%	0.001%
59	10.622	2976	2980	2981	rBV2	638	383	0.02%	0.002%
60	10.696	3001	3003	3008	rVB4	600	394	0.02%	0.002%
61	10.722	3008	3011	3013	rBV2	533	410	0.02%	0.002%
62	10.763	3023	3024	3025	rBV	396	103	0.00%	0.001%
63	10.779	3025	3029	3034	rVV6	1196	1278	0.05%	0.007%
64	10.934	3075	3077	3080	rVB3	895	468	0.02%	0.003%
65	10.950	3080	3082	3086	rVB2	697	404	0.02%	0.002%
66	10.972	3086	3089	3090	rBV	618	261	0.01%	0.001%
67	11.114	3132	3133	3135	rBV	415	203	0.01%	0.001%
68	11.178	3143	3153	3187	rBV	1066700	1696121	70.49%	9.666%
69	11.554	3258	3270	3300	rBV	1061865	1730889	71.94%	9.864%
70	11.889	3370	3374	3379	rBV7	1053	1158	0.05%	0.007%
71	12.053	3423	3425	3430	rVB4	1375	926	0.04%	0.005%
72	12.467	3551	3554	3555	rBV2	646	338	0.01%	0.002%
73	12.480	3555	3558	3562	rVV4	887	709	0.03%	0.004%
74	12.535	3572	3575	3578	rBV2	891	761	0.03%	0.004%
75	13.123	3756	3758	3759	rBV	679	302	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037705.D
Acq On : 01 Oct 2024 16:00
Operator : SY/MD
Sample : P4203-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

Sum of corrected areas: 17547681




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037705.D
Acq On : 01 Oct 2024 16:00
Operator : SY/MD
Sample : P4203-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

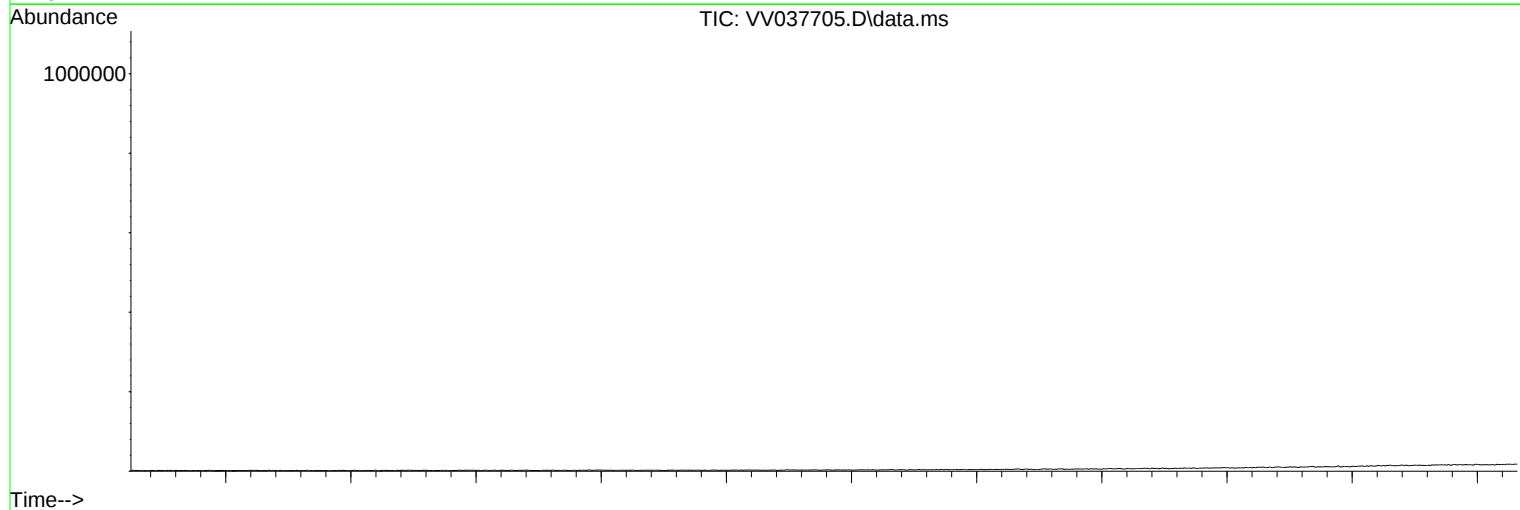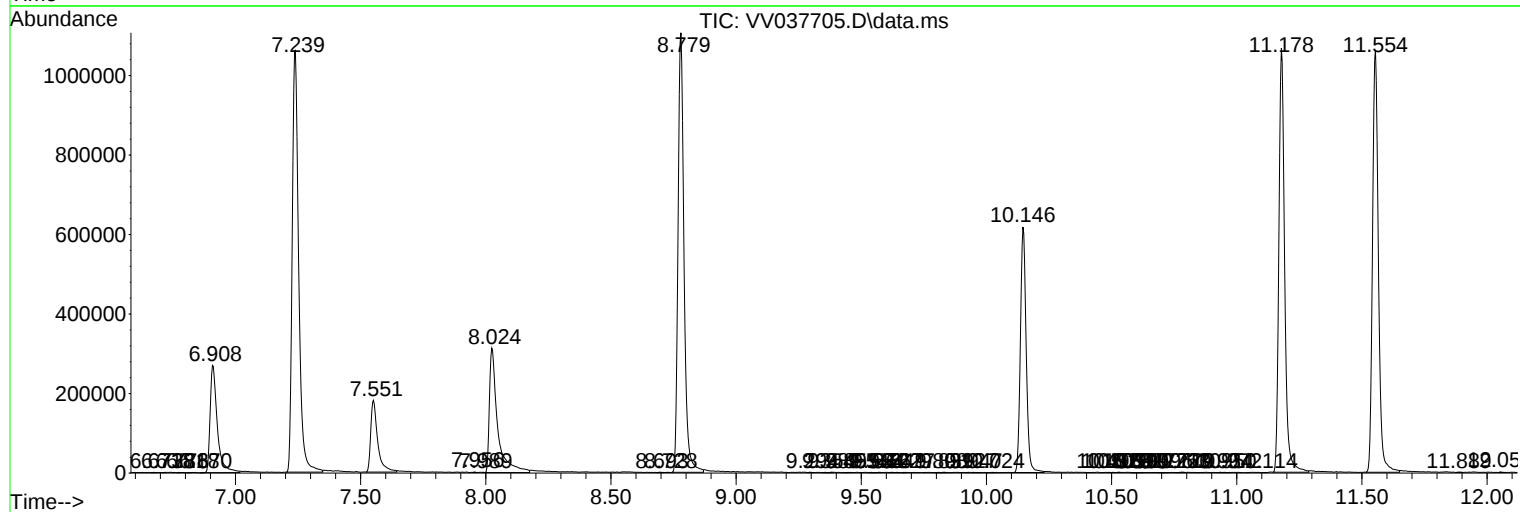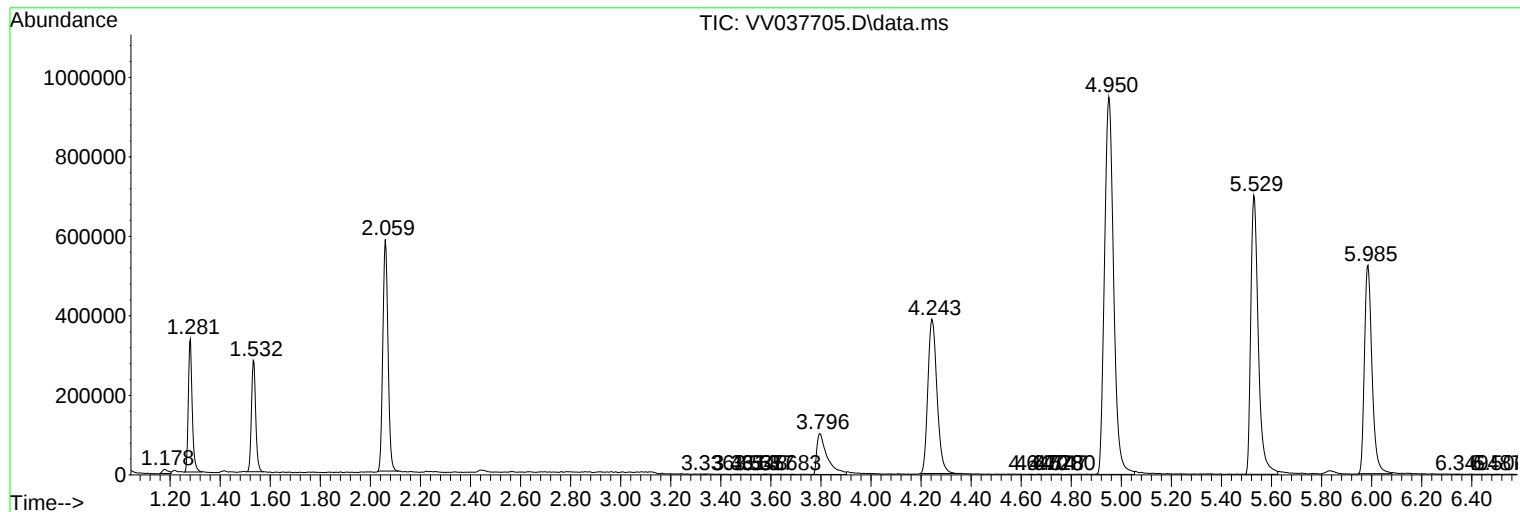

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037705.D
Acq On : 01 Oct 2024 16:00
Operator : SY/MD
Sample : P4203-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037705.D
Acq On : 01 Oct 2024 16:00
Operator : SY/MD
Sample : P4203-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc