

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037707.D
 Acq On : 01 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4205-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	52	rBV	12255	19121	0.81%	0.110%
2	1.278	68	74	93	rVB	326650	356179	15.08%	2.057%
3	1.532	146	153	168	rVB	277252	322348	13.65%	1.862%
4	2.060	307	317	337	rVB	575187	831232	35.20%	4.800%
5	3.442	745	747	749	rBV2	435	232	0.01%	0.001%
6	3.510	766	768	771	rBV2	672	295	0.01%	0.002%
7	3.555	779	782	788	rBV3	781	856	0.04%	0.005%
8	3.587	790	792	794	rVB2	553	204	0.01%	0.001%
9	3.603	794	797	799	rBV2	789	489	0.02%	0.003%
10	3.651	810	812	816	rBV2	581	374	0.02%	0.002%
11	3.677	819	820	823	rBV2	380	214	0.01%	0.001%
12	3.793	848	856	896	rBV	103776	302257	12.80%	1.745%
13	4.243	979	996	1027	rBV	385891	984489	41.69%	5.685%
14	4.651	1121	1123	1125	rVB3	806	353	0.01%	0.002%
15	4.664	1125	1127	1130	rBV2	685	446	0.02%	0.003%
16	4.728	1142	1147	1148	rBV	689	562	0.02%	0.003%
17	4.780	1160	1163	1167	rBV4	521	504	0.02%	0.003%
18	4.863	1184	1189	1190	rBV2	674	585	0.02%	0.003%
19	4.950	1200	1216	1245	rBV2	935201	2361577	100.00%	13.638%
20	5.400	1353	1356	1359	rBV3	736	507	0.02%	0.003%
21	5.462	1373	1375	1376	rBV2	499	204	0.01%	0.001%
22	5.529	1385	1396	1426	rBV	683896	1408531	59.64%	8.134%
23	5.986	1525	1538	1567	rBV	525217	1100207	46.59%	6.354%
24	6.252	1618	1621	1622	rBV2	924	497	0.02%	0.003%
25	6.404	1664	1668	1670	rBV3	593	512	0.02%	0.003%
26	6.474	1688	1690	1693	rVB2	632	288	0.01%	0.002%
27	6.490	1693	1695	1698	rBV3	790	590	0.02%	0.003%
28	6.609	1729	1732	1734	rBV2	522	296	0.01%	0.002%
29	6.651	1740	1745	1748	rVB4	646	578	0.02%	0.003%
30	6.677	1751	1753	1755	rBV4	703	334	0.01%	0.002%
31	6.725	1765	1768	1770	rVB3	501	286	0.01%	0.002%
32	6.760	1777	1779	1783	rVB3	795	342	0.01%	0.002%
33	6.815	1793	1796	1798	rBV2	501	321	0.01%	0.002%
34	6.873	1811	1814	1815	rBV2	665	404	0.02%	0.002%
35	6.908	1816	1825	1859	rVV	264574	517086	21.90%	2.986%
36	7.240	1916	1928	1958	rBV	1045035	1863632	78.91%	10.762%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037707.D
 Acq On : 01 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4205-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2051	rBV2	177419	338477	14.33%	1.955%
38	7.969	2152	2155	2158	rBV4	669	491	0.02%	0.003%
39	8.024	2164	2172	2219	rBV2	323714	724479	30.68%	4.184%
40	8.465	2306	2309	2311	rBV4	876	612	0.03%	0.004%
41	8.780	2395	2407	2440	rBV	1069809	1792079	75.88%	10.349%
42	9.194	2533	2536	2539	rVB5	820	519	0.02%	0.003%
43	9.211	2539	2541	2543	rBV2	561	267	0.01%	0.002%
44	9.265	2554	2558	2559	rBV4	414	274	0.01%	0.002%
45	9.352	2580	2585	2587	rBV3	603	502	0.02%	0.003%
46	9.371	2590	2591	2594	rVB2	721	335	0.01%	0.002%
47	9.394	2594	2598	2601	rBV5	1015	841	0.04%	0.005%
48	9.432	2608	2610	2615	rVB4	1028	678	0.03%	0.004%
49	9.493	2627	2629	2632	rBV2	309	207	0.01%	0.001%
50	9.522	2636	2638	2641	rBV3	877	495	0.02%	0.003%
51	9.545	2643	2645	2647	rVB2	511	220	0.01%	0.001%
52	9.593	2653	2660	2664	rVB6	462	614	0.03%	0.004%
53	9.670	2678	2684	2687	rVB5	849	866	0.04%	0.005%
54	9.693	2687	2691	2693	rBV3	752	620	0.03%	0.004%
55	9.767	2711	2714	2716	rBV3	799	455	0.02%	0.003%
56	9.789	2719	2721	2725	rVB3	773	411	0.02%	0.002%
57	9.812	2725	2728	2730	rBV3	602	286	0.01%	0.002%
58	9.841	2734	2737	2740	rVB	614	272	0.01%	0.002%
59	9.857	2740	2742	2746	rBV	417	399	0.02%	0.002%
60	9.924	2760	2763	2765	rBV	592	415	0.02%	0.002%
61	9.956	2769	2773	2776	rBV3	350	262	0.01%	0.002%
62	10.002	2780	2787	2788	rBV2	794	735	0.03%	0.004%
63	10.030	2793	2796	2798	rBV2	457	293	0.01%	0.002%
64	10.146	2820	2832	2855	rBV	622615	991310	41.98%	5.725%
65	10.358	2895	2898	2902	rVB3	903	570	0.02%	0.003%
66	10.384	2902	2906	2907	rBV2	810	580	0.02%	0.003%
67	10.429	2917	2920	2923	rBV3	540	308	0.01%	0.002%
68	10.448	2923	2926	2929	rVV4	483	338	0.01%	0.002%
69	10.484	2935	2937	2942	rVB4	1142	803	0.03%	0.005%
70	10.519	2942	2948	2951	rBV4	918	879	0.04%	0.005%
71	10.538	2952	2954	2957	rVB3	895	464	0.02%	0.003%
72	10.596	2968	2972	2974	rBV4	959	868	0.04%	0.005%
73	10.632	2981	2983	2984	rBV	636	225	0.01%	0.001%
74	10.641	2984	2986	2990	rVV3	402	214	0.01%	0.001%
75	10.667	2991	2994	2997	rVB2	620	354	0.01%	0.002%
76	10.690	2998	3001	3004	rBV2	772	585	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037707.D
 Acq On : 01 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4205-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.751	3016	3020	3022	rBV3	834	562	0.02%	0.003%
78	10.776	3027	3028	3032	rBV3	531	439	0.02%	0.003%
79	10.866	3051	3056	3058	rBV4	926	938	0.04%	0.005%
80	10.889	3061	3063	3069	rVB4	662	567	0.02%	0.003%
81	10.928	3072	3075	3077	rBV2	576	298	0.01%	0.002%
82	10.947	3077	3081	3084	rBV	462	337	0.01%	0.002%
83	10.969	3084	3088	3092	rBV4	532	518	0.02%	0.003%
84	10.995	3095	3096	3101	rBV3	735	467	0.02%	0.003%
85	11.095	3124	3127	3128	rBV2	421	247	0.01%	0.001%
86	11.130	3134	3138	3140	rBV2	1088	885	0.04%	0.005%
87	11.178	3142	3153	3183	rBV	1011556	1645639	69.68%	9.503%
88	11.551	3258	3269	3306	rBV	1040770	1719751	72.82%	9.931%
89	11.995	3405	3407	3412	rBV4	608	525	0.02%	0.003%
90	12.040	3420	3421	3423	rBV	565	292	0.01%	0.002%
91	12.120	3443	3446	3449	rBV4	760	611	0.03%	0.004%
92	12.153	3453	3456	3459	rBV3	1113	646	0.03%	0.004%
93	12.262	3488	3490	3491	rBV	636	263	0.01%	0.002%
94	12.394	3528	3531	3534	rVB3	547	377	0.02%	0.002%
95	12.497	3561	3563	3564	rBV2	719	281	0.01%	0.002%
96	12.654	3610	3612	3614	rBV2	560	292	0.01%	0.002%
97	12.754	3642	3643	3647	rBV4	503	342	0.01%	0.002%
98	13.088	3744	3747	3748	rBV2	451	276	0.01%	0.002%
99	13.400	3840	3844	3849	rBV4	889	908	0.04%	0.005%
100	13.442	3855	3857	3860	rBV3	774	402	0.02%	0.002%




Sum of corrected areas: 17316397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037707.D
Acq On : 01 Oct 2024 16:43
Operator : SY/MD
Sample : P4205-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

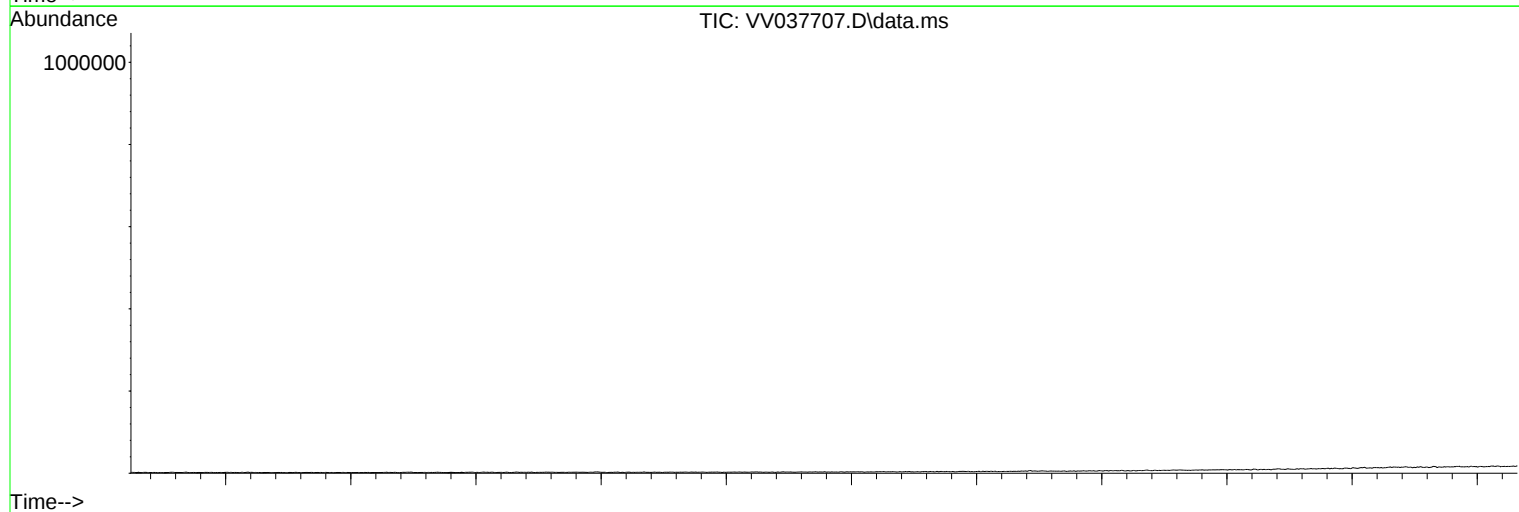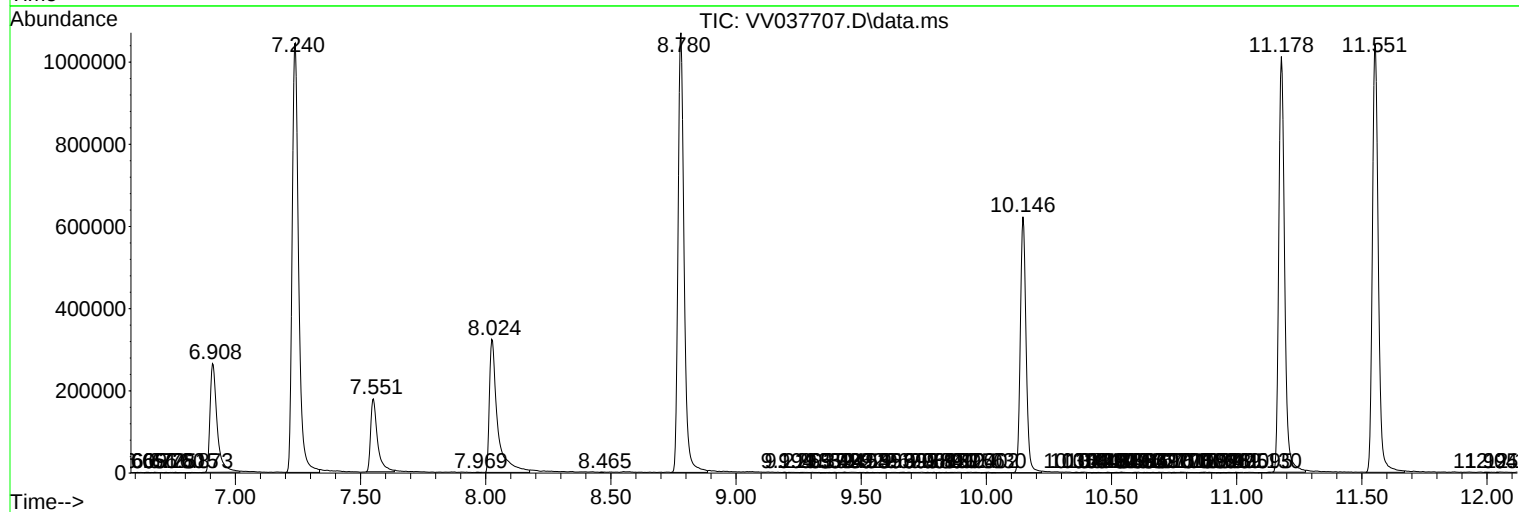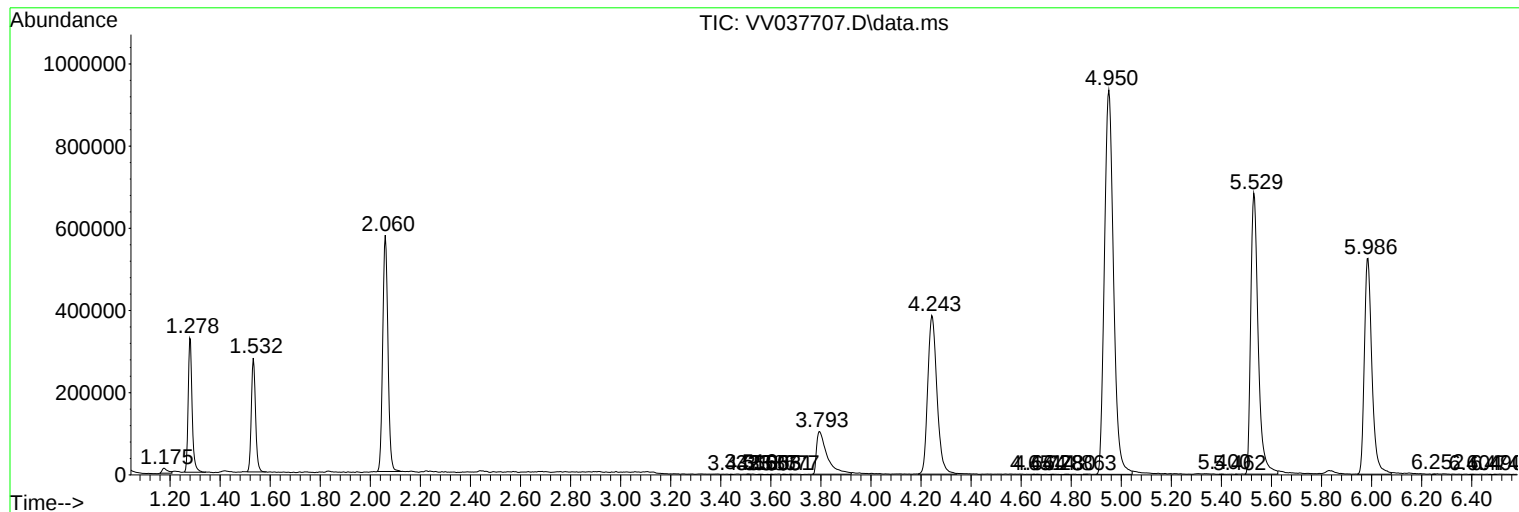

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037707.D
Acq On : 01 Oct 2024 16:43
Operator : SY/MD
Sample : P4205-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037707.D
Acq On : 01 Oct 2024 16:43
Operator : SY/MD
Sample : P4205-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc