

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037708.D
 Acq On : 01 Oct 2024 17:05
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	51	rBV	10835	17996	0.78%	0.105%
2	1.278	68	74	91	rVB	317860	346309	14.93%	2.016%
3	1.532	146	153	166	rVB	271286	320515	13.81%	1.866%
4	2.060	308	317	336	rVB	559652	804163	34.66%	4.681%
5	3.404	733	735	742	rVB3	907	858	0.04%	0.005%
6	3.455	746	751	753	rBV3	696	606	0.03%	0.004%
7	3.581	787	790	792	rVV2	515	286	0.01%	0.002%
8	3.642	805	809	812	rBV4	718	556	0.02%	0.003%
9	3.693	821	825	826	rBV2	573	314	0.01%	0.002%
10	3.741	836	840	842	rBV3	511	403	0.02%	0.002%
11	3.796	848	857	888	rBV	102281	290618	12.53%	1.692%
12	4.243	975	996	1026	rBV	374099	967369	41.70%	5.631%
13	4.625	1112	1115	1119	rBV3	910	741	0.03%	0.004%
14	4.671	1127	1129	1131	rBV	473	238	0.01%	0.001%
15	4.732	1145	1148	1152	rBV3	527	426	0.02%	0.002%
16	4.879	1191	1194	1197	rBV4	602	429	0.02%	0.002%
17	4.950	1200	1216	1246	rBV2	913721	2320099	100.00%	13.506%
18	5.265	1311	1314	1316	rBV3	782	465	0.02%	0.003%
19	5.317	1328	1330	1335	rBV6	1208	1195	0.05%	0.007%
20	5.378	1347	1349	1353	rVB3	1029	583	0.03%	0.003%
21	5.404	1353	1357	1359	rBV4	1319	1001	0.04%	0.006%
22	5.433	1364	1366	1370	rBV3	286	236	0.01%	0.001%
23	5.484	1376	1382	1383	rBV5	788	577	0.02%	0.003%
24	5.529	1385	1396	1430	rBV	709681	1472133	63.45%	8.569%
25	5.986	1526	1538	1573	rBV	511326	1059058	45.65%	6.165%
26	6.233	1612	1615	1616	rBV3	1064	449	0.02%	0.003%
27	6.278	1626	1629	1630	rBV3	701	356	0.02%	0.002%
28	6.381	1658	1661	1663	rBV4	616	373	0.02%	0.002%
29	6.426	1672	1675	1676	rBV	434	279	0.01%	0.002%
30	6.461	1684	1686	1687	rBV	739	284	0.01%	0.002%
31	6.539	1708	1710	1713	rBV2	408	261	0.01%	0.002%
32	6.574	1719	1721	1724	rVB2	789	424	0.02%	0.002%
33	6.590	1724	1726	1728	rVB	505	215	0.01%	0.001%
34	6.600	1728	1729	1734	rBV3	441	321	0.01%	0.002%
35	6.651	1743	1745	1746	rBV	482	220	0.01%	0.001%
36	6.690	1755	1757	1760	rBV3	520	330	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037708.D
 Acq On : 01 Oct 2024 17:05
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.722	1764	1767	1769	rBV2	503	347	0.01%	0.002%
38	6.754	1775	1777	1779	rBV2	701	356	0.02%	0.002%
39	6.767	1779	1781	1784	rVV4	749	540	0.02%	0.003%
40	6.796	1788	1790	1792	rBV	657	325	0.01%	0.002%
41	6.809	1792	1794	1797	rVV4	628	313	0.01%	0.002%
42	6.908	1815	1825	1852	rBV	259518	506322	21.82%	2.947%
43	7.240	1917	1928	1952	rBV	1016808	1809864	78.01%	10.535%
44	7.551	2016	2025	2051	rBV	173098	328230	14.15%	1.911%
45	7.825	2108	2110	2114	rVB4	1705	733	0.03%	0.004%
46	8.024	2161	2172	2207	rBV2	310142	680993	29.35%	3.964%
47	8.712	2384	2386	2389	rVB2	647	374	0.02%	0.002%
48	8.735	2389	2393	2395	rBV5	691	669	0.03%	0.004%
49	8.780	2396	2407	2443	rBV	1126491	1861660	80.24%	10.837%
50	9.275	2559	2561	2565	rBV3	407	222	0.01%	0.001%
51	9.333	2575	2579	2580	rBV3	635	522	0.02%	0.003%
52	9.371	2589	2591	2594	rVB3	663	335	0.01%	0.002%
53	9.432	2607	2610	2611	rBV	467	240	0.01%	0.001%
54	9.513	2632	2635	2636	rBV2	528	249	0.01%	0.001%
55	9.603	2658	2663	2665	rBV3	909	720	0.03%	0.004%
56	9.696	2689	2692	2695	rVB2	672	461	0.02%	0.003%
57	9.735	2700	2704	2705	rBV3	566	277	0.01%	0.002%
58	9.799	2722	2724	2730	rVB4	508	467	0.02%	0.003%
59	9.831	2731	2734	2736	rBV2	345	249	0.01%	0.001%
60	9.915	2758	2760	2764	rVB3	824	467	0.02%	0.003%
61	9.940	2766	2768	2774	rVB5	599	588	0.03%	0.003%
62	9.969	2775	2777	2781	rVB3	611	385	0.02%	0.002%
63	9.995	2781	2785	2786	rBV2	627	336	0.01%	0.002%
64	10.046	2795	2801	2805	rBV4	694	747	0.03%	0.004%
65	10.146	2819	2832	2861	rBV	607562	974198	41.99%	5.671%
66	10.320	2883	2886	2888	rBV2	742	559	0.02%	0.003%
67	10.387	2905	2907	2908	rBV	530	222	0.01%	0.001%
68	10.484	2933	2937	2943	rVB7	1064	1180	0.05%	0.007%
69	10.516	2943	2947	2949	rBV2	958	750	0.03%	0.004%
70	10.600	2971	2973	2978	rVB3	487	254	0.01%	0.001%
71	10.628	2978	2982	2984	rBV4	558	441	0.02%	0.003%
72	10.728	3009	3013	3016	rBV	667	539	0.02%	0.003%
73	10.757	3020	3022	3026	rBV3	492	403	0.02%	0.002%
74	10.783	3026	3030	3033	rBV3	1328	1202	0.05%	0.007%
75	10.834	3043	3046	3048	rBV2	380	227	0.01%	0.001%
76	10.850	3048	3051	3053	rBV2	555	297	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037708.D
 Acq On : 01 Oct 2024 17:05
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.911	3064	3070	3073	rBV4	668	428	0.02%	0.002%
78	11.001	3095	3098	3099	rBV	507	249	0.01%	0.001%
79	11.040	3106	3110	3114	rBV4	503	441	0.02%	0.003%
80	11.091	3123	3126	3129	rBV2	876	715	0.03%	0.004%
81	11.127	3134	3137	3138	rBV	772	394	0.02%	0.002%
82	11.136	3138	3140	3142	rBV3	708	300	0.01%	0.002%
83	11.178	3142	3153	3185	rBV	1079590	1710895	73.74%	9.959%
84	11.554	3258	3270	3302	rBV	1026074	1669160	71.94%	9.716%
85	12.082	3431	3434	3436	rBV2	679	371	0.02%	0.002%
86	12.098	3437	3439	3441	rBV2	769	400	0.02%	0.002%
87	12.143	3451	3453	3456	rVB2	679	371	0.02%	0.002%
88	12.162	3456	3459	3461	rBV2	735	396	0.02%	0.002%
89	12.442	3543	3546	3548	rBV3	684	432	0.02%	0.003%
90	12.706	3625	3628	3631	rBV4	883	705	0.03%	0.004%
91	12.773	3646	3649	3651	rBV4	644	425	0.02%	0.002%
92	12.850	3670	3673	3676	rBV3	859	715	0.03%	0.004%
93	12.892	3684	3686	3689	rVB3	791	341	0.01%	0.002%
94	12.911	3689	3692	3696	rBV4	968	936	0.04%	0.005%
95	13.056	3735	3737	3739	rBV2	582	274	0.01%	0.002%
96	13.111	3752	3754	3757	rVB3	716	308	0.01%	0.002%
97	13.207	3782	3784	3788	rBV3	810	556	0.02%	0.003%
98	13.384	3836	3839	3841	rBV2	763	636	0.03%	0.004%
99	13.416	3847	3849	3852	rBV2	822	501	0.02%	0.003%
100	14.895	4307	4309	4312	rBV4	1449	903	0.04%	0.005%

Sum of corrected areas: 17178801




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037708.D
Acq On : 01 Oct 2024 17:05
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

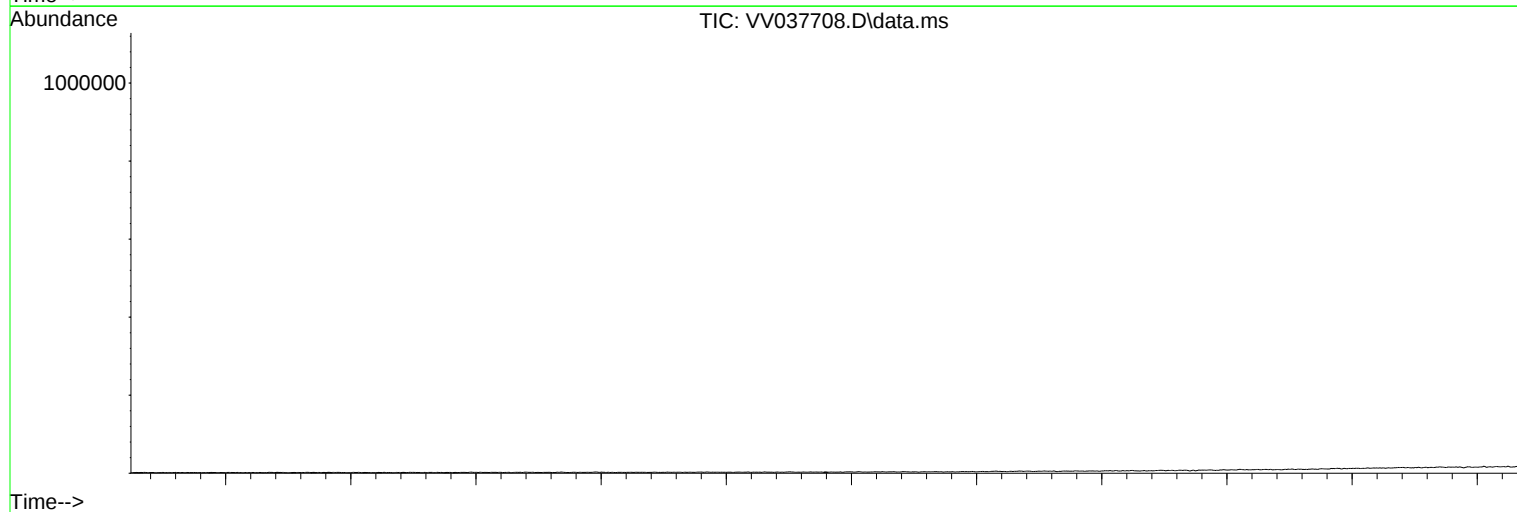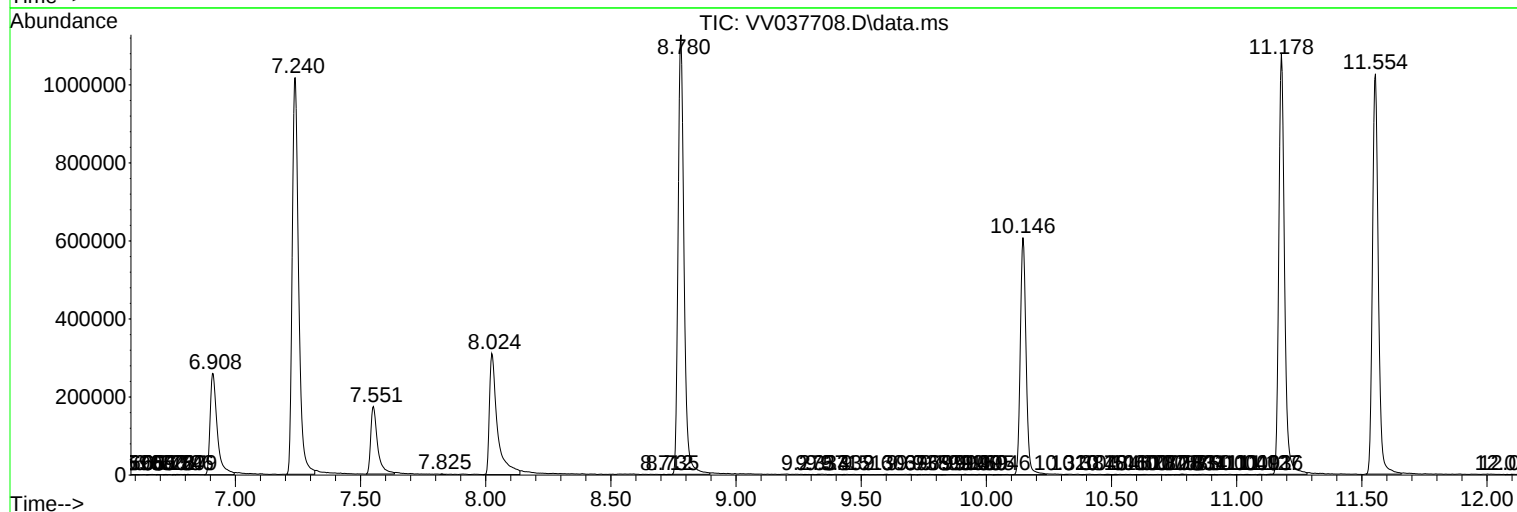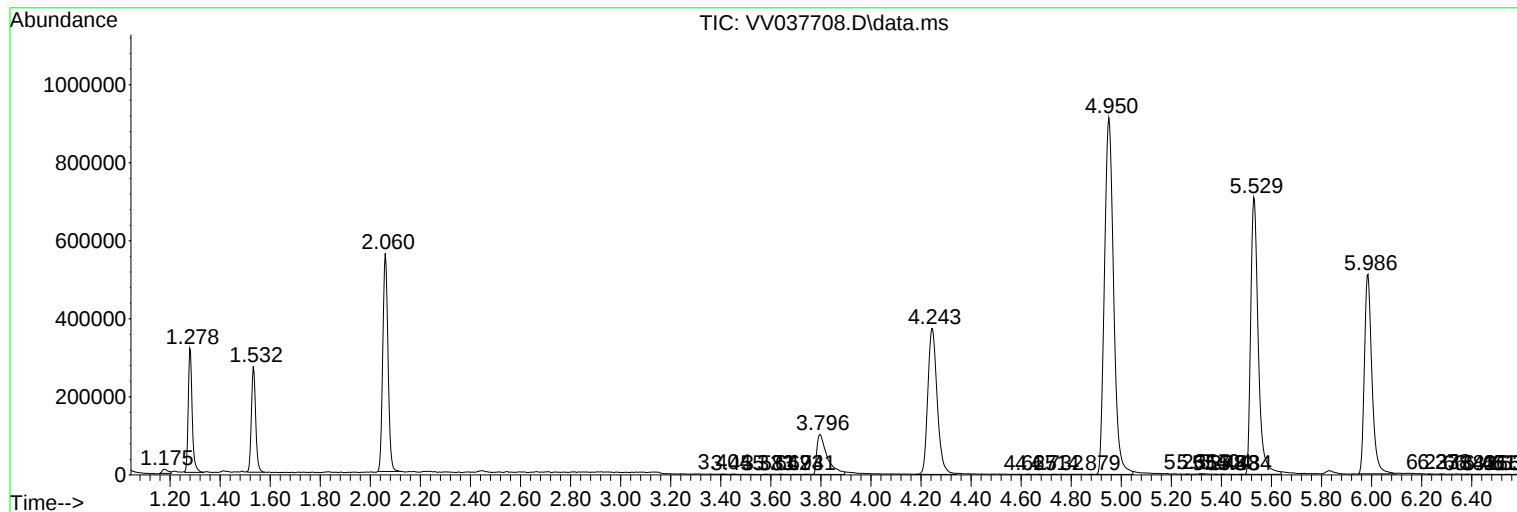

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037708.D
Acq On : 01 Oct 2024 17:05
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037708.D
Acq On : 01 Oct 2024 17:05
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------