

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037709.D
 Acq On : 01 Oct 2024 17:27
 Operator : SY/MD
 Sample : P4237-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV	12639	20802	0.89%	0.121%
2	1.278	67	74	91	rVB	318635	342672	14.60%	2.001%
3	1.532	145	153	166	rVB	270838	321604	13.70%	1.878%
4	2.060	306	317	331	rBV	562845	807840	34.42%	4.716%
5	3.233	680	682	686	rVB5	847	524	0.02%	0.003%
6	3.471	754	756	761	rVB4	995	806	0.03%	0.005%
7	3.548	775	780	783	rBV5	965	841	0.04%	0.005%
8	3.645	805	810	812	rBV3	971	822	0.04%	0.005%
9	3.699	826	827	831	rVB3	811	445	0.02%	0.003%
10	3.796	848	857	889	rBV2	102587	287400	12.25%	1.678%
11	4.095	947	950	954	rBV3	622	506	0.02%	0.003%
12	4.243	976	996	1024	rBV	384009	971846	41.41%	5.674%
13	4.375	1035	1037	1044	rVB7	1637	1597	0.07%	0.009%
14	4.449	1056	1060	1063	rBV4	871	653	0.03%	0.004%
15	4.516	1077	1081	1084	rBV4	1129	692	0.03%	0.004%
16	4.564	1094	1096	1101	rVB5	1002	853	0.04%	0.005%
17	4.600	1101	1107	1111	rBV3	746	954	0.04%	0.006%
18	4.712	1137	1142	1143	rBV2	796	488	0.02%	0.003%
19	4.806	1165	1171	1174	rBV4	855	886	0.04%	0.005%
20	4.950	1200	1216	1253	rBV2	918393	2346974	100.00%	13.702%
21	5.320	1328	1331	1335	rBV4	1165	971	0.04%	0.006%
22	5.529	1384	1396	1428	rBV	684057	1411203	60.13%	8.239%
23	5.831	1480	1490	1502	rBV5	8624	19432	0.83%	0.113%
24	5.912	1513	1515	1518	rBV4	835	618	0.03%	0.004%
25	5.982	1525	1537	1569	rBV	512878	1079172	45.98%	6.300%
26	6.429	1675	1676	1681	rVB4	1203	816	0.03%	0.005%
27	6.494	1694	1696	1699	rVB3	883	520	0.02%	0.003%
28	6.548	1708	1713	1716	rVB4	622	558	0.02%	0.003%
29	6.603	1726	1730	1733	rBV5	579	556	0.02%	0.003%
30	6.731	1766	1770	1774	rBV3	1035	1053	0.04%	0.006%
31	6.908	1814	1825	1855	rBV	260435	508958	21.69%	2.971%
32	7.188	1907	1912	1915	rBV3	804	640	0.03%	0.004%
33	7.236	1916	1927	1953	rBV	1026354	1820085	77.55%	10.626%
34	7.551	2015	2025	2054	rBV2	170133	331958	14.14%	1.938%
35	7.902	2129	2134	2137	rBV5	1185	1198	0.05%	0.007%
36	7.921	2137	2140	2146	rVB4	901	909	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037709.D
 Acq On : 01 Oct 2024 17:27
 Operator : SY/MD
 Sample : P4237-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.966	2151	2154	2158	rBV3	1025	671	0.03%	0.004%
38	8.024	2163	2172	2214	rBV2	313026	705541	30.06%	4.119%
39	8.336	2267	2269	2272	rBV3	1241	872	0.04%	0.005%
40	8.471	2308	2311	2316	rBV5	672	748	0.03%	0.004%
41	8.522	2325	2327	2330	rVB4	1110	590	0.03%	0.003%
42	8.548	2332	2335	2337	rBV4	821	567	0.02%	0.003%
43	8.674	2370	2374	2376	rBV3	652	554	0.02%	0.003%
44	8.780	2392	2407	2451	rBV	1085008	1802165	76.79%	10.521%
45	9.037	2485	2487	2490	rBV3	903	527	0.02%	0.003%
46	9.239	2546	2550	2553	rVB3	605	453	0.02%	0.003%
47	9.326	2574	2577	2580	rVB4	856	465	0.02%	0.003%
48	9.355	2580	2586	2587	rBV4	549	554	0.02%	0.003%
49	9.519	2635	2637	2641	rVB3	888	455	0.02%	0.003%
50	9.664	2679	2682	2685	rBV4	742	577	0.02%	0.003%
51	9.789	2714	2721	2723	rBV5	784	854	0.04%	0.005%
52	9.882	2743	2750	2752	rBV3	632	600	0.03%	0.004%
53	9.899	2752	2755	2758	rBV2	881	469	0.02%	0.003%
54	9.953	2768	2772	2775	rVB2	631	466	0.02%	0.003%
55	10.014	2785	2791	2795	rVV4	841	940	0.04%	0.005%
56	10.146	2820	2832	2859	rBV	606550	976233	41.60%	5.699%
57	10.323	2884	2887	2892	rVB4	1256	958	0.04%	0.006%
58	10.349	2892	2895	2898	rBV4	1122	784	0.03%	0.005%
59	10.400	2908	2911	2916	rVB3	776	696	0.03%	0.004%
60	10.429	2916	2920	2922	rBV4	672	465	0.02%	0.003%
61	10.474	2930	2934	2936	rVV3	736	528	0.02%	0.003%
62	10.651	2985	2989	2995	rBV5	771	761	0.03%	0.004%
63	10.677	2995	2997	3004	rVB3	804	741	0.03%	0.004%
64	10.770	3021	3026	3027	rBV3	892	784	0.03%	0.005%
65	10.783	3027	3030	3039	rVB5	504	679	0.03%	0.004%
66	11.053	3108	3114	3115	rBV4	798	618	0.03%	0.004%
67	11.178	3141	3153	3184	rBV	1015909	1631580	69.52%	9.525%
68	11.458	3237	3240	3243	rVB4	866	543	0.02%	0.003%
69	11.554	3256	3270	3301	rBV	1030765	1685098	71.80%	9.838%
70	11.882	3368	3372	3375	rBV4	1127	868	0.04%	0.005%
71	11.911	3379	3381	3388	rBV6	948	839	0.04%	0.005%
72	11.956	3392	3395	3399	rBV4	677	600	0.03%	0.004%
73	12.008	3408	3411	3415	rBV6	1227	1198	0.05%	0.007%
74	12.333	3505	3512	3515	rBV5	1536	1829	0.08%	0.011%
75	12.432	3539	3543	3546	rBV3	627	529	0.02%	0.003%
76	12.535	3568	3575	3577	rBV5	527	598	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037709.D
 Acq On : 01 Oct 2024 17:27
 Operator : SY/MD
 Sample : P4237-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.561	3581	3583	3587	rVV4	736	499	0.02%	0.003%
78	12.583	3587	3590	3593	rVV3	708	596	0.03%	0.003%
79	12.603	3594	3596	3600	rVV3	1001	647	0.03%	0.004%
80	12.632	3603	3605	3612	rVB4	791	518	0.02%	0.003%
81	12.661	3612	3614	3618	rBV4	697	444	0.02%	0.003%
82	13.033	3726	3730	3732	rBV2	1038	670	0.03%	0.004%
83	13.223	3785	3789	3794	rVB4	1607	1348	0.06%	0.008%
84	13.300	3809	3813	3817	rBV4	742	820	0.03%	0.005%
85	13.323	3817	3820	3823	rBV4	969	643	0.03%	0.004%
86	13.342	3823	3826	3829	rVV2	940	814	0.03%	0.005%
87	13.413	3846	3848	3852	rBV3	595	457	0.02%	0.003%
88	13.461	3861	3863	3865	rVV2	854	512	0.02%	0.003%
89	13.480	3867	3869	3872	rVV2	1109	742	0.03%	0.004%
90	13.513	3876	3879	3883	rVB2	574	493	0.02%	0.003%
91	13.779	3960	3962	3968	rVB5	783	581	0.02%	0.003%
92	14.143	4072	4075	4078	rVB3	1168	883	0.04%	0.005%
93	14.168	4078	4083	4084	rBV3	1190	846	0.04%	0.005%
94	14.220	4095	4099	4103	rVB3	955	878	0.04%	0.005%
95	14.329	4131	4133	4138	rVB2	844	590	0.03%	0.003%
96	14.355	4138	4141	4145	rBV4	726	643	0.03%	0.004%
97	14.558	4200	4204	4207	rBV4	870	849	0.04%	0.005%
98	14.615	4220	4222	4224	rBV2	804	540	0.02%	0.003%
99	14.731	4256	4258	4261	rVB4	1058	486	0.02%	0.003%
100	14.834	4286	4290	4292	rBV3	991	804	0.03%	0.005%

Sum of corrected areas: 17129152




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037709.D
Acq On : 01 Oct 2024 17:27
Operator : SY/MD
Sample : P4237-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

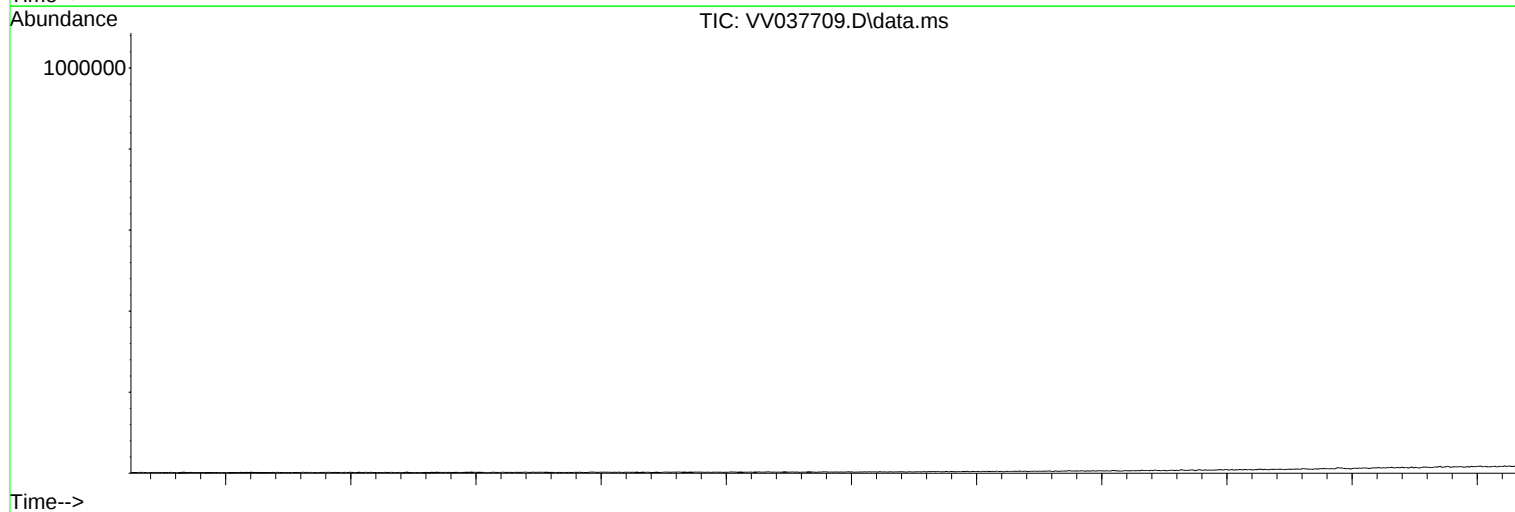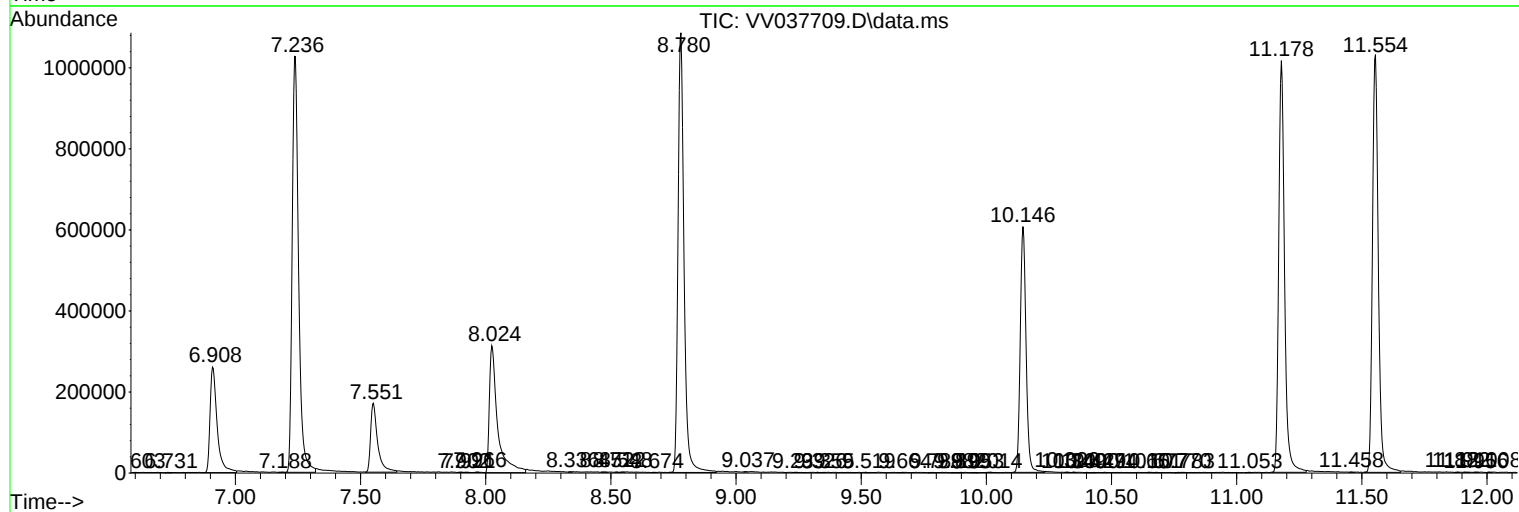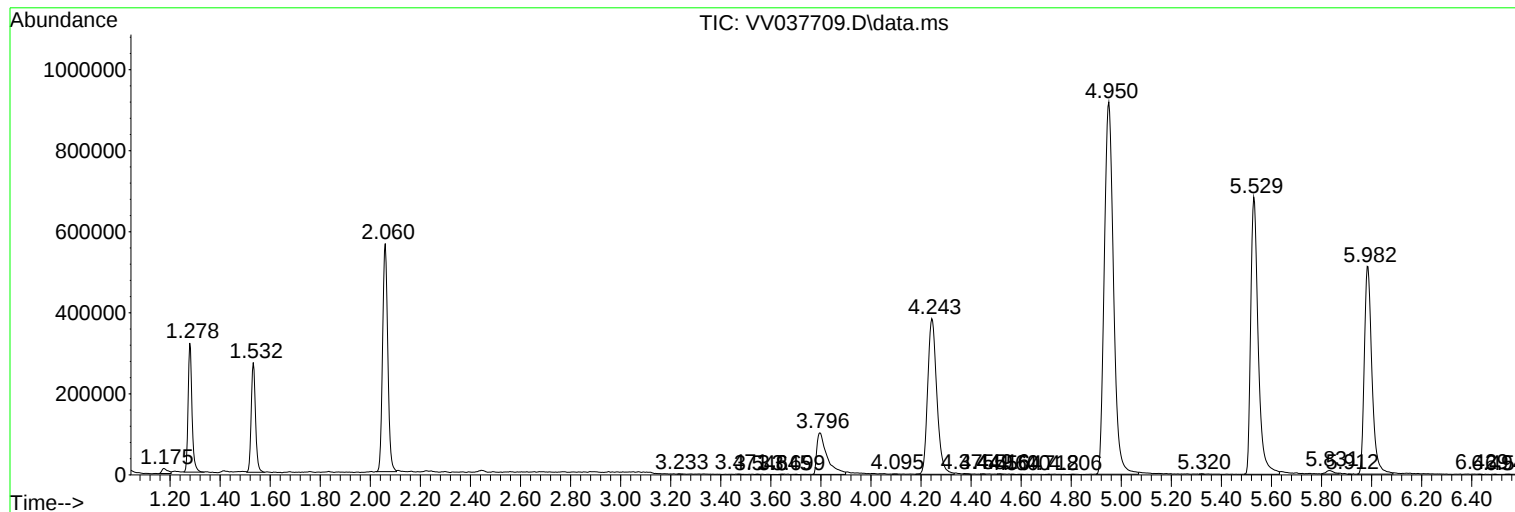

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037709.D
Acq On : 01 Oct 2024 17:27
Operator : SY/MD
Sample : P4237-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037709.D
Acq On : 01 Oct 2024 17:27
Operator : SY/MD
Sample : P4237-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------