

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037710.D
 Acq On : 01 Oct 2024 17:48
 Operator : SY/MD
 Sample : P4238-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	50	rBV	13220	20901	0.89%	0.122%
2	1.214	51	54	62	rVB2	5504	8337	0.35%	0.049%
3	1.278	67	74	89	rVV	317898	348531	14.80%	2.038%
4	1.532	145	153	165	rBV	270183	315161	13.38%	1.843%
5	2.059	307	317	331	rBV	562647	810566	34.42%	4.740%
6	3.394	729	732	735	rBV4	978	596	0.03%	0.003%
7	3.471	751	756	761	rBV5	481	488	0.02%	0.003%
8	3.500	761	765	768	rBV3	935	694	0.03%	0.004%
9	3.738	835	839	847	rVB4	718	726	0.03%	0.004%
10	3.796	847	857	899	rBV	100778	301095	12.79%	1.761%
11	4.075	941	944	947	rBV3	741	464	0.02%	0.003%
12	4.243	980	996	1028	rVV	381725	971337	41.25%	5.680%
13	4.426	1049	1053	1058	rVB4	565	486	0.02%	0.003%
14	4.461	1061	1064	1066	rBV3	699	447	0.02%	0.003%
15	4.545	1087	1090	1095	rBV4	628	610	0.03%	0.004%
16	4.574	1097	1099	1102	rVB3	1035	603	0.03%	0.004%
17	4.850	1184	1185	1190	rVB	744	478	0.02%	0.003%
18	4.883	1190	1195	1198	rBV2	860	591	0.03%	0.003%
19	4.950	1198	1216	1256	rBV2	921735	2354603	100.00%	13.769%
20	5.236	1303	1305	1312	rVB6	1009	935	0.04%	0.005%
21	5.371	1344	1347	1357	rVB7	848	1221	0.05%	0.007%
22	5.416	1357	1361	1365	rBV4	765	691	0.03%	0.004%
23	5.529	1385	1396	1435	rVV	670909	1400957	59.50%	8.192%
24	5.831	1480	1490	1505	rBV6	7920	19450	0.83%	0.114%
25	5.937	1521	1523	1525	rBV2	889	550	0.02%	0.003%
26	5.985	1525	1538	1572	rVV	521457	1089495	46.27%	6.371%
27	6.133	1582	1584	1587	rVB4	1374	562	0.02%	0.003%
28	6.227	1611	1613	1618	rVV5	863	556	0.02%	0.003%
29	6.249	1618	1620	1626	rVB6	876	854	0.04%	0.005%
30	6.278	1627	1629	1632	rBV4	814	482	0.02%	0.003%
31	6.317	1636	1641	1644	rVB3	644	522	0.02%	0.003%
32	6.471	1686	1689	1694	rVV4	841	732	0.03%	0.004%
33	6.526	1703	1706	1709	rBV3	974	715	0.03%	0.004%
34	6.760	1777	1779	1782	rVB2	1033	544	0.02%	0.003%
35	6.808	1789	1794	1796	rBV4	657	517	0.02%	0.003%
36	6.908	1813	1825	1851	rBV	256045	507883	21.57%	2.970%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037710.D
 Acq On : 01 Oct 2024 17:48
 Operator : SY/MD
 Sample : P4238-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.239	1916	1928	1961	rBV	1033243	1837023	78.02%	10.742%
38	7.551	2015	2025	2052	rBV	177756	338122	14.36%	1.977%
39	7.982	2153	2159	2163	rBV6	621	660	0.03%	0.004%
40	8.024	2163	2172	2221	rBV2	311193	705638	29.97%	4.126%
41	8.516	2322	2325	2329	rBV5	608	504	0.02%	0.003%
42	8.651	2365	2367	2369	rVV2	942	458	0.02%	0.003%
43	8.673	2371	2374	2381	rVB4	849	751	0.03%	0.004%
44	8.779	2395	2407	2441	rBV	1064881	1764796	74.95%	10.320%
45	9.114	2508	2511	2514	rVB4	948	507	0.02%	0.003%
46	9.143	2518	2520	2525	rVB3	807	634	0.03%	0.004%
47	9.165	2525	2527	2533	rVB4	1014	916	0.04%	0.005%
48	9.197	2533	2537	2540	rBV4	1401	1031	0.04%	0.006%
49	9.268	2557	2559	2563	rVB2	815	564	0.02%	0.003%
50	9.326	2575	2577	2580	rVB4	869	456	0.02%	0.003%
51	9.406	2599	2602	2605	rVB4	1303	962	0.04%	0.006%
52	9.451	2613	2616	2620	rVB3	1160	782	0.03%	0.005%
53	9.474	2620	2623	2626	rBV2	675	515	0.02%	0.003%
54	9.496	2626	2630	2633	rBV4	659	474	0.02%	0.003%
55	9.564	2645	2651	2655	rBV5	804	908	0.04%	0.005%
56	9.612	2664	2666	2673	rVB5	808	654	0.03%	0.004%
57	9.828	2731	2733	2736	rBV2	810	446	0.02%	0.003%
58	9.873	2746	2747	2752	rVB	855	477	0.02%	0.003%
59	9.985	2778	2782	2783	rBV3	706	495	0.02%	0.003%
60	10.021	2789	2793	2797	rBV3	715	604	0.03%	0.004%
61	10.146	2820	2832	2857	rBV	606529	972925	41.32%	5.689%
62	10.281	2869	2874	2878	rVB8	1128	1129	0.05%	0.007%
63	10.323	2884	2887	2891	rVB3	684	505	0.02%	0.003%
64	10.458	2925	2929	2930	rVV3	679	447	0.02%	0.003%
65	10.509	2943	2945	2950	rVV2	593	470	0.02%	0.003%
66	10.583	2963	2968	2972	rVB3	598	634	0.03%	0.004%
67	10.651	2985	2989	2991	rBV5	1118	643	0.03%	0.004%
68	10.747	3017	3019	3025	rBV2	500	491	0.02%	0.003%
69	10.786	3026	3031	3036	rVB7	635	678	0.03%	0.004%
70	11.178	3142	3153	3183	rBV	986302	1598450	67.89%	9.347%
71	11.384	3213	3217	3219	rBV3	868	758	0.03%	0.004%
72	11.554	3258	3270	3304	rBV	1053163	1683856	71.51%	9.846%
73	11.866	3362	3367	3370	rBV5	1257	1212	0.05%	0.007%
74	11.927	3382	3386	3390	rVB5	1005	813	0.03%	0.005%
75	12.136	3448	3451	3455	rBV3	776	479	0.02%	0.003%
76	12.213	3469	3475	3478	rBV5	1211	1202	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037710.D
 Acq On : 01 Oct 2024 17:48
 Operator : SY/MD
 Sample : P4238-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.303	3500	3503	3507	rVB3	638	536	0.02%	0.003%
78	12.410	3533	3536	3539	rVV4	1106	560	0.02%	0.003%
79	12.554	3578	3581	3587	rVB4	1032	850	0.04%	0.005%
80	12.792	3652	3655	3658	rBV4	607	435	0.02%	0.003%
81	12.869	3677	3679	3682	rBV	517	440	0.02%	0.003%
82	12.895	3684	3687	3690	rVV3	998	628	0.03%	0.004%
83	12.921	3693	3695	3701	rBV3	604	505	0.02%	0.003%
84	12.969	3707	3710	3712	rVB3	889	513	0.02%	0.003%
85	13.088	3744	3747	3751	rBV2	768	712	0.03%	0.004%
86	13.291	3806	3810	3813	rBV3	684	545	0.02%	0.003%
87	13.583	3898	3901	3905	rVB4	706	554	0.02%	0.003%
88	13.631	3912	3916	3919	rBV2	646	528	0.02%	0.003%
89	13.676	3927	3930	3933	rBV3	981	727	0.03%	0.004%
90	13.747	3949	3952	3956	rBV3	720	456	0.02%	0.003%
91	13.773	3956	3960	3963	rBV6	1016	924	0.04%	0.005%
92	13.982	4023	4025	4028	rBV2	849	691	0.03%	0.004%
93	14.091	4055	4059	4061	rBV2	727	531	0.02%	0.003%
94	14.143	4072	4075	4078	rBV3	702	549	0.02%	0.003%
95	14.188	4085	4089	4090	rBV2	840	581	0.02%	0.003%
96	14.461	4171	4174	4175	rBV2	928	531	0.02%	0.003%
97	14.779	4269	4273	4275	rBV4	1016	654	0.03%	0.004%
98	14.869	4298	4301	4303	rBV3	1447	755	0.03%	0.004%
99	14.895	4306	4309	4311	rBV3	1170	846	0.04%	0.005%
100	15.249	4416	4419	4422	rBV4	837	667	0.03%	0.004%




Sum of corrected areas: 17101167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037710.D
Acq On : 01 Oct 2024 17:48
Operator : SY/MD
Sample : P4238-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

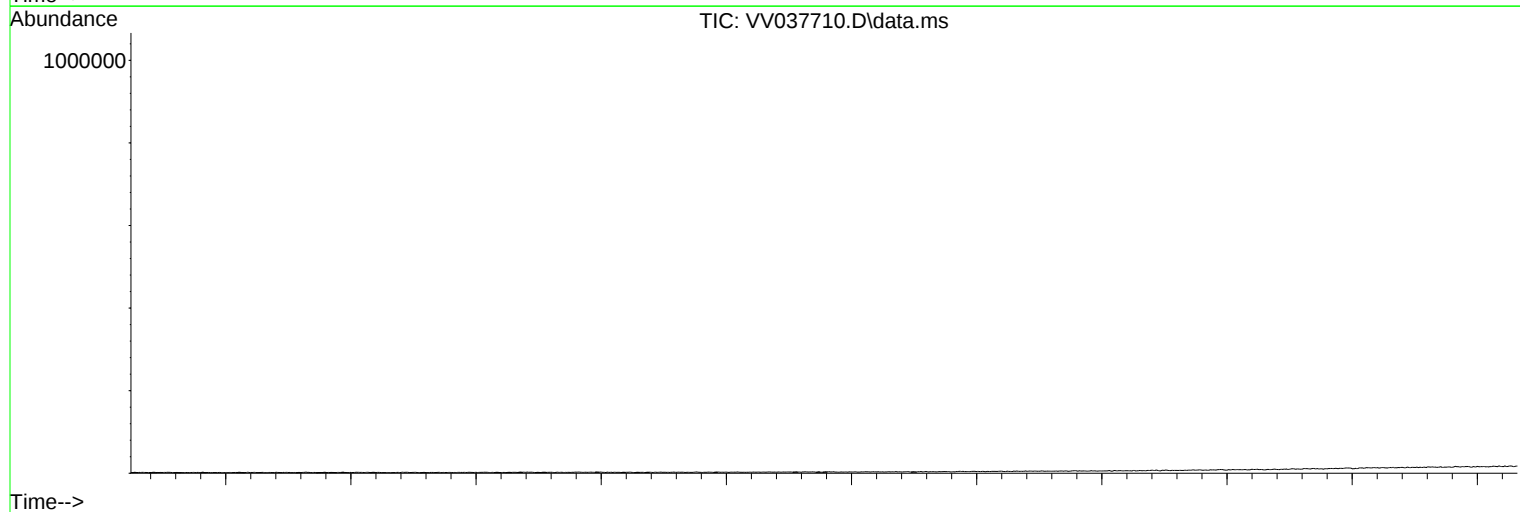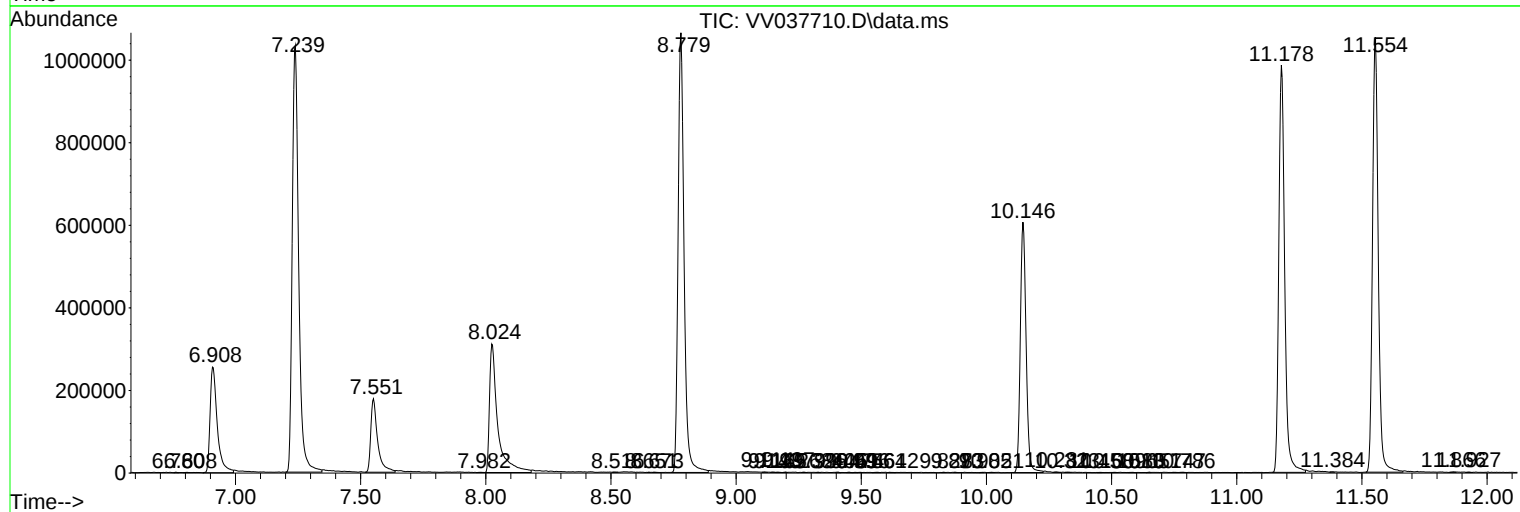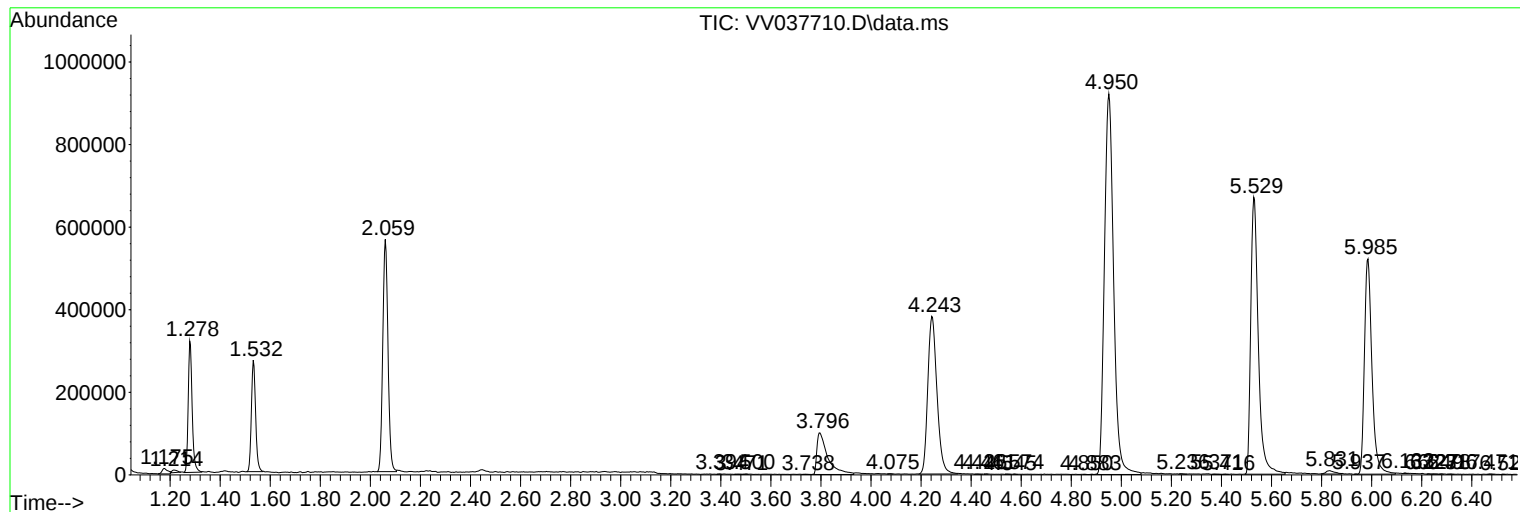

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037710.D
Acq On : 01 Oct 2024 17:48
Operator : SY/MD
Sample : P4238-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037710.D
Acq On : 01 Oct 2024 17:48
Operator : SY/MD
Sample : P4238-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------