
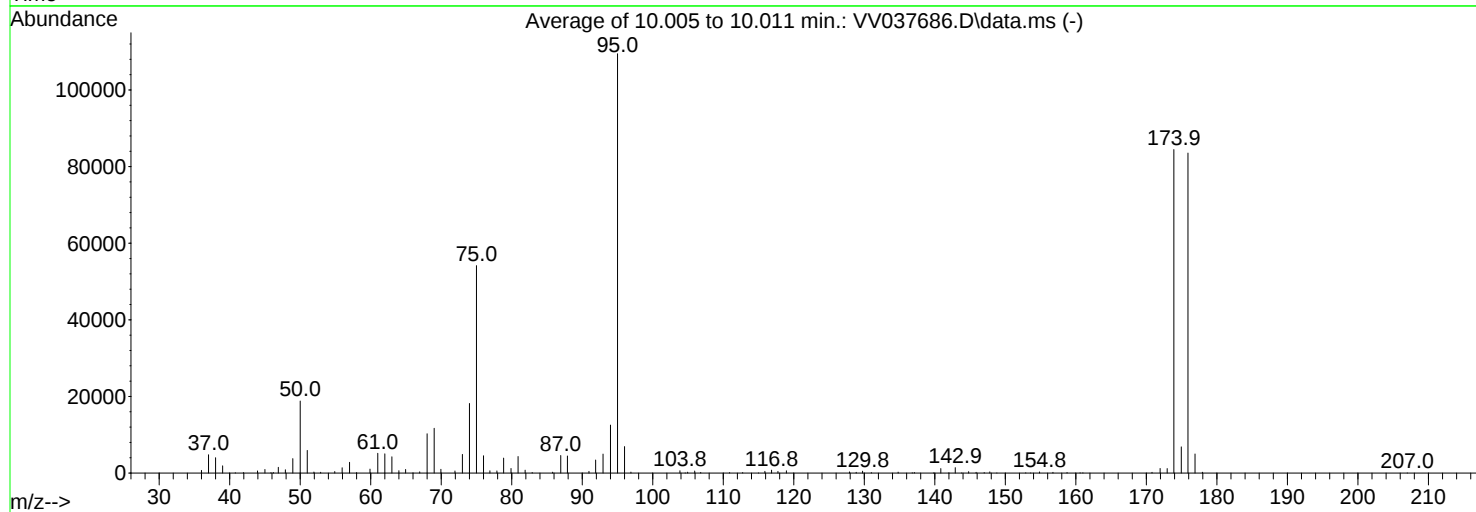


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037686.D
Acq On : 01 Oct 2024 08:23
Operator : SY/MD
Sample : BFB384
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB384

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Tue Oct 01 04:32:07 2024

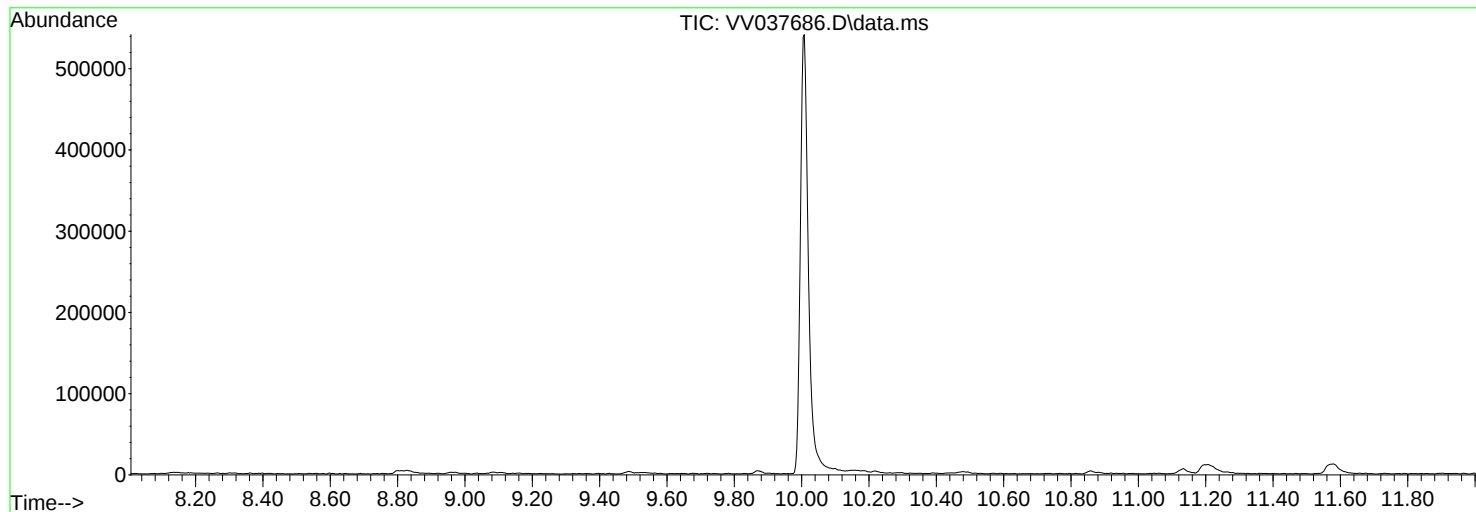

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	18811	PASS
75	95	30	80	49.5	54149	PASS
95	95	100	100	100.0	109459	PASS
96	95	5	9	6.3	6914	PASS
173	174	0.00	2	1.4	1177	PASS
174	95	50	120	77.1	84445	PASS
175	174	5	9	8.1	6839	PASS
176	174	95	105	98.9	83541	PASS
177	176	5	10	6.0	4984	PASS

m/z	Abundance
36.00	145.0
39.90	348.0
43.90	779.0
76.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
36.00	951.0
37.00	4759.0
38.00	4351.0
39.00	1928.0
40.00	337.0
42.00	136.0
44.00	1402.0
45.00	911.0
45.80	134.0
46.20	196.0
46.90	1528.0
47.90	871.0
48.90	4022.0
50.00	19240.0
51.00	6284.0
52.10	267.0
52.90	251.0
54.90	407.0
55.90	1431.0
57.00	2967.0
58.00	186.0
59.90	1109.0
61.00	5551.0
62.00	5136.0
63.00	4541.0
64.00	757.0
65.00	949.0
66.90	362.0
68.00	10654.0
69.00	11890.0
69.90	901.0
72.00	618.0
73.00	5120.0
74.00	19248.0
75.00	56248.0
76.00	4665.0
76.90	846.0
77.80	753.0
78.90	4148.0
79.90	1314.0
80.90	4436.0
81.80	805.0
82.90	155.0
85.80	283.0
87.00	4776.0
87.90	4706.0
91.00	502.0
91.90	3408.0
93.00	5257.0
94.00	12702.0
95.00	112552.0
96.00	6918.0
96.90	196.0
103.90	595.0
104.90	281.0
106.00	571.0
106.80	183.0
110.80	123.0
112.80	123.0
115.00	126.0
115.90	499.0
116.90	771.0
117.70	457.0
118.90	598.0
127.90	388.0
128.80	221.0
129.80	551.0
131.00	133.0
134.90	341.0
136.80	285.0
139.80	121.0
140.80	1307.0
142.90	1462.0
144.80	399.0
145.90	203.0
147.00	167.0
147.80	296.0
148.80	110.0
154.90	364.0
156.80	155.0
158.70	145.0
161.00	119.0
170.80	266.0
172.00	1305.0
172.90	1144.0
173.90	85416.0
174.90	6881.0
175.90	83488.0
176.90	5192.0
178.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
36.00	803.0
37.00	5006.0
38.00	4119.0
39.00	1936.0
40.00	356.0
40.80	116.0
42.00	136.0
44.00	1413.0
45.00	1001.0
46.20	200.0
46.90	1567.0
47.90	895.0
49.00	3757.0
50.00	19440.0
51.00	6171.0
51.90	286.0
52.90	206.0
54.90	411.0
56.00	1421.0
57.00	2934.0
58.00	157.0
59.90	1079.0
61.00	5260.0
62.00	5181.0
63.00	4363.0
64.00	633.0
64.90	968.0
67.00	325.0
68.00	10519.0
69.00	12129.0
70.00	1021.0
72.00	568.0
73.00	5080.0
74.00	18712.0
75.00	55656.0
76.00	4675.0
76.90	809.0
77.90	538.0
78.90	3977.0
79.90	1259.0
80.90	4454.0
81.90	744.0
82.90	167.0
85.80	258.0
87.00	4626.0
87.90	4657.0
91.00	469.0
91.90	3557.0
92.90	5217.0
94.00	12771.0
95.00	113168.0
96.00	7045.0
96.90	275.0
103.80	642.0
104.90	259.0
105.90	560.0
106.80	192.0
110.90	112.0
112.80	149.0
115.90	493.0
116.80	770.0
117.70	451.0
118.90	648.0
127.90	300.0
128.80	204.0
129.80	497.0
131.00	135.0
134.80	217.0
137.10	234.0
140.80	1202.0
142.90	1488.0
144.80	386.0
145.90	224.0
147.00	140.0
147.80	327.0
152.90	104.0
154.80	307.0
156.70	200.0
158.70	163.0
160.60	101.0
161.00	125.0
170.80	186.0
172.00	1222.0
173.00	1227.0
173.90	87328.0
175.00	7068.0
175.90	86456.0
176.90	5116.0
177.90	143.0
178.00	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
36.00	770.0
37.00	4615.0
38.00	3545.0
39.00	1828.0
39.90	349.0
40.80	148.0
41.90	118.0
44.00	1222.0
45.00	896.0
45.90	168.0
46.90	1419.0
47.90	823.0
49.00	3528.0
50.00	17752.0
51.00	5287.0
51.90	275.0
52.90	175.0
54.90	397.0
56.00	1318.0
57.00	2526.0
59.90	927.0
61.00	4691.0
62.00	4764.0
63.00	3839.0
64.00	508.0
64.90	922.0
66.00	107.0
67.00	277.0
68.00	9596.0
69.00	11053.0
70.00	1040.0
71.90	468.0
73.00	4435.0
74.00	16552.0
75.00	50544.0
76.00	4249.0
76.90	640.0
78.00	407.0
78.80	3618.0
79.90	1051.0
80.90	4087.0
82.00	733.0
82.90	142.0
85.80	201.0
86.90	4359.0
87.90	4013.0
90.80	387.0
91.90	3255.0
92.90	4431.0
94.00	12119.0
95.00	102656.0
96.00	6778.0
96.90	323.0
103.80	600.0
104.60	135.0
105.00	195.0
105.90	501.0
106.80	170.0
111.00	125.0
112.70	123.0
115.90	414.0
116.80	760.0
117.80	403.0
119.00	580.0
127.90	261.0
128.90	172.0
129.70	447.0
131.00	121.0
134.70	215.0
137.10	213.0
140.90	1025.0
142.00	184.0
142.90	1305.0
143.80	122.0
144.80	330.0
145.80	192.0
147.00	117.0
147.80	302.0
152.90	120.0
153.60	104.0
154.80	230.0
156.70	234.0
158.80	156.0
160.60	137.0
170.90	139.0
171.90	1100.0
173.00	1160.0
173.90	80592.0
175.00	6567.0
175.90	80680.0
176.90	4645.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

178.10
207.00

122.0
125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384