

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
 Data File : VV037716.D
 Acq On : 02 Oct 2024 13:17
 Operator : SY/MD
 Sample : P4239-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 03 05:56:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 03 05:55:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	684003	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	675443	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	313356	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	180242	30.018	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	60.040%
7) Chloroethane-d5	1.532	69	173095	37.139	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.280%
11) 1,1-Dichloroethene-d2	2.060	65	90402	36.037	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.080%
21) 2-Butanone-d5	3.786	46	184643	86.335	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.340%
24) Chloroform-d	4.236	84	463206	43.361	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.720%
26) 1,2-Dichloroethane-d4	4.931	65	281956	45.093	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.180%
32) Benzene-d6	4.947	84	871821	41.248	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.500%
36) 1,2-Dichloropropane-d6	5.979	67	290317	43.136	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.280%
41) Toluene-d8	7.233	98	751013	39.186	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.380%#
43) trans-1,3-Dichloroprop...	7.548	79	123035	39.352	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.700%
47) 2-Hexanone-d5	8.021	63	105884	74.505	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.500%
56) 1,1,2,2-Tetrachloroeth...	10.143	84	328057	41.950	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.900%
66) 1,2-Dichlorobenzene-d4	11.551	152	312460	47.321	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.640%
Target Compounds						
13) Acetone	2.111	43	59692	28.472	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037716.D
Acq On : 02 Oct 2024 13:17
Operator : SY/MD
Sample : P4239-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 03 05:56:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 03 05:55:19 2024
Response via : Initial Calibration

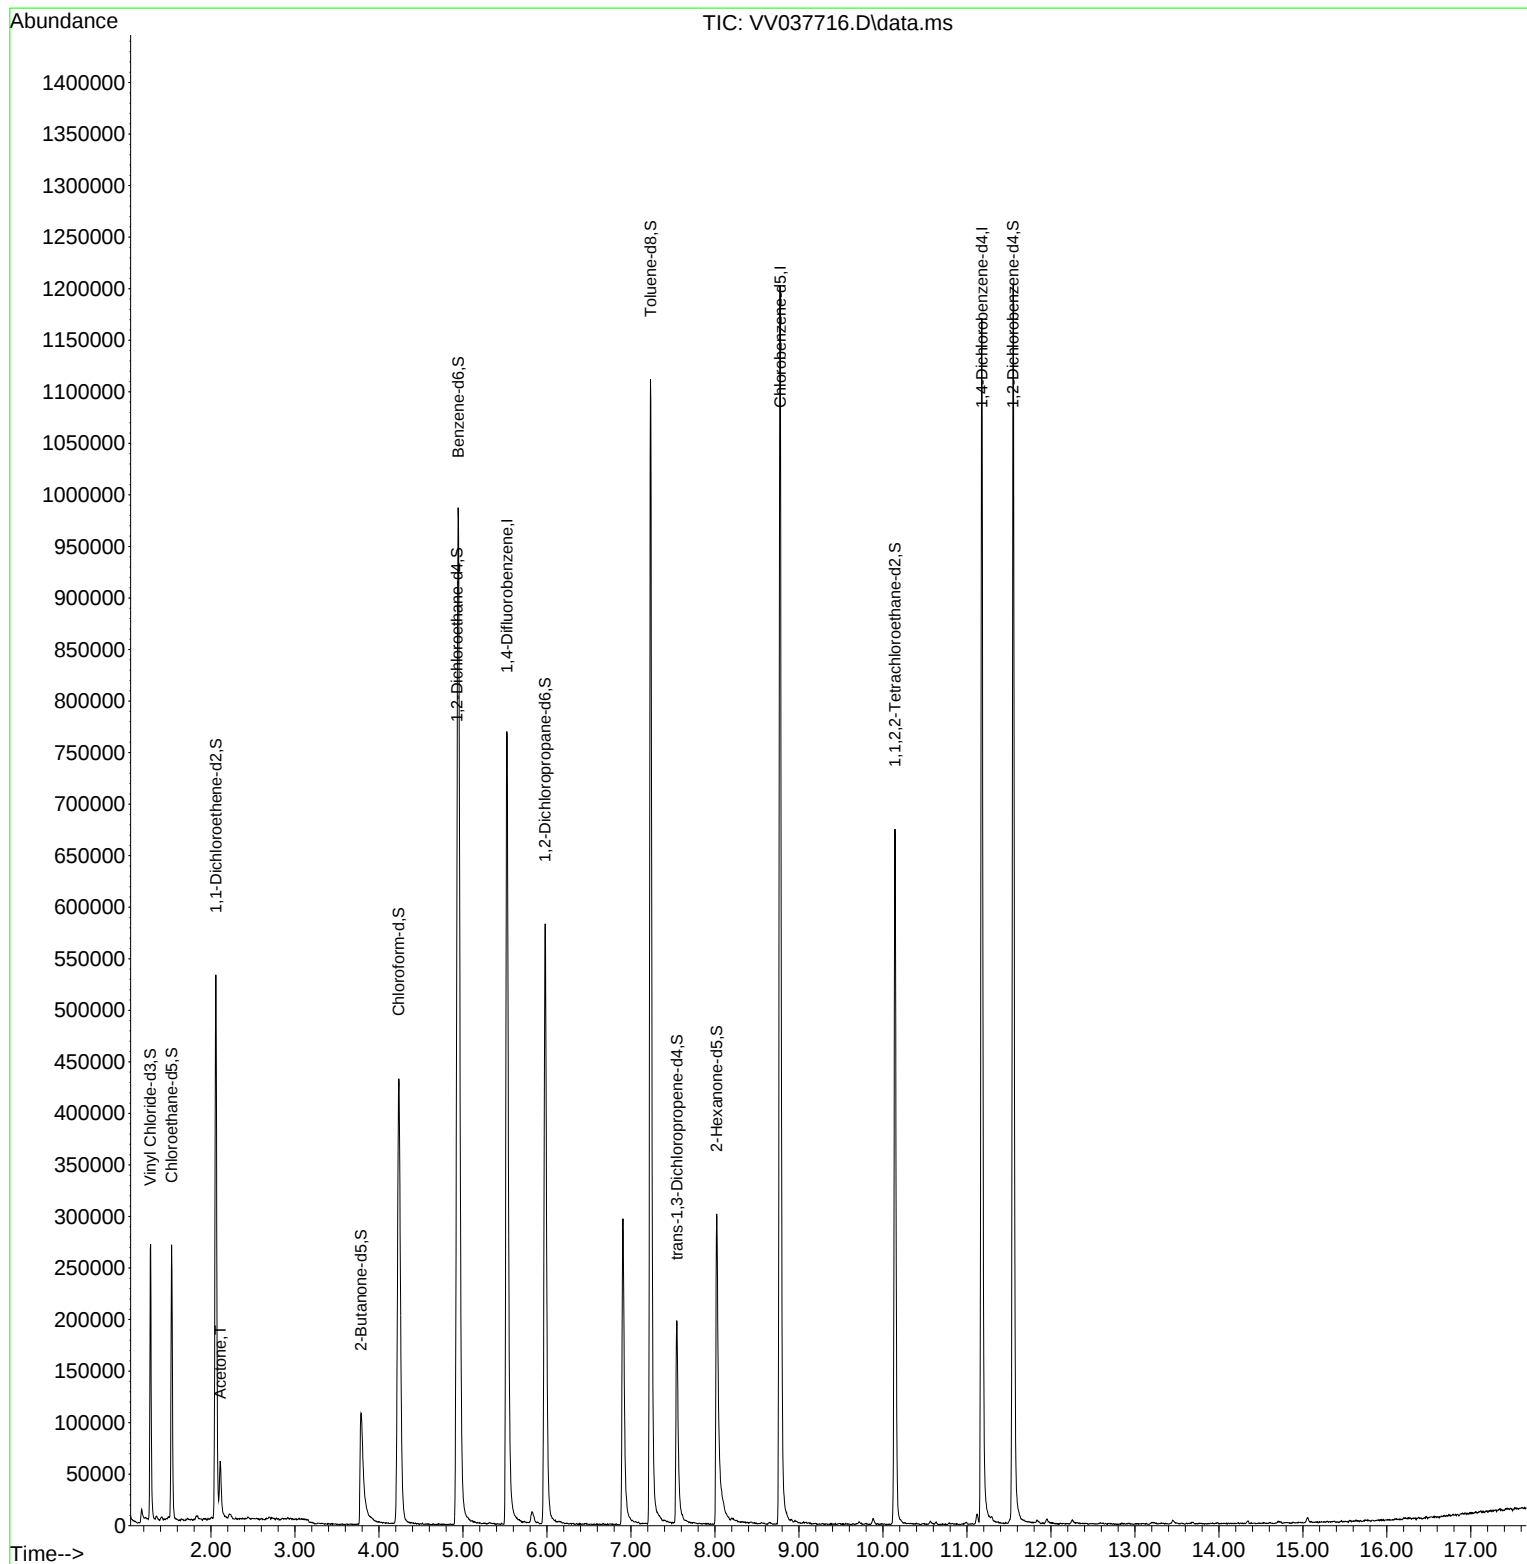

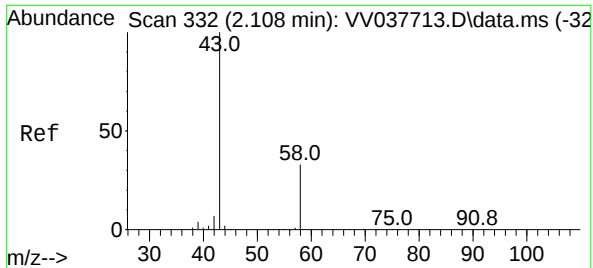

#13
 Acetone
 Concen: 28.472 ug/L
 RT: 2.111 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV037716.D
 Acq: 02 Oct 2024 13:17

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 43 Resp: 59692
 Ion Ratio Lower Upper
 43 100
 58 32.0 0.0 66.6

