

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
 Data File : VV037716.D
 Acq On : 02 Oct 2024 13:17
 Operator : SY/MD
 Sample : P4239-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	52	rBV	12845	21618	0.85%	0.116%
2	1.282	68	75	92	rVB	266846	290545	11.44%	1.559%
3	1.532	146	153	165	rVB	265411	307139	12.09%	1.648%
4	2.060	307	317	327	rBV	526038	766992	30.20%	4.115%
5	3.433	741	744	746	rBV4	1023	733	0.03%	0.004%
6	3.510	764	768	770	rVB3	623	460	0.02%	0.002%
7	3.519	770	771	773	rBV	308	135	0.01%	0.001%
8	3.536	773	776	778	rBV5	454	291	0.01%	0.002%
9	3.548	778	780	781	rBV	346	186	0.01%	0.001%
10	3.590	791	793	795	rVB2	382	158	0.01%	0.001%
11	3.613	795	800	803	rBV3	704	588	0.02%	0.003%
12	3.648	807	811	813	rBV2	485	458	0.02%	0.002%
13	3.725	833	835	837	rBV2	398	249	0.01%	0.001%
14	3.741	837	840	845	rBV4	539	438	0.02%	0.002%
15	3.786	845	854	891	rBV	107949	325518	12.82%	1.746%
16	4.236	979	994	1029	rVB	430665	1086133	42.76%	5.827%
17	4.587	1101	1103	1105	rBV	400	154	0.01%	0.001%
18	4.635	1116	1118	1119	rBV	381	119	0.00%	0.001%
19	4.651	1119	1123	1126	rVB4	985	798	0.03%	0.004%
20	4.680	1126	1132	1135	rBV5	616	585	0.02%	0.003%
21	4.699	1135	1138	1140	rBV2	623	396	0.02%	0.002%
22	4.770	1157	1160	1161	rBV	583	353	0.01%	0.002%
23	4.799	1167	1169	1170	rBV2	347	158	0.01%	0.001%
24	4.841	1177	1182	1183	rBV3	612	471	0.02%	0.003%
25	4.944	1198	1214	1248	rBV2	986379	2540044	100.00%	13.628%
26	5.458	1371	1374	1380	rBV6	1369	1357	0.05%	0.007%
27	5.523	1383	1394	1430	rBV	769022	1601561	63.05%	8.593%
28	5.979	1523	1536	1563	rBV	581600	1196124	47.09%	6.417%
29	6.355	1650	1653	1657	rVB4	1015	644	0.03%	0.003%
30	6.381	1659	1661	1662	rBV	803	289	0.01%	0.002%
31	6.391	1662	1664	1665	rVV2	704	230	0.01%	0.001%
32	6.416	1669	1672	1673	rBV2	581	326	0.01%	0.002%
33	6.452	1680	1683	1684	rBV3	871	497	0.02%	0.003%
34	6.548	1710	1713	1715	rBV2	613	371	0.01%	0.002%
35	6.561	1715	1717	1724	rVB4	947	769	0.03%	0.004%
36	6.593	1724	1727	1731	rVB3	1001	717	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037716.D
Acq On : 02 Oct 2024 13:17
Operator : SY/MD
Sample : P4239-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

37	6.619	1731	1735	1738	rBV4	525	550	0.02%	0.003%
38	6.667	1746	1750	1751	rBV3	970	479	0.02%	0.003%
39	6.696	1757	1759	1760	rBV	598	203	0.01%	0.001%
40	6.722	1763	1767	1769	rBV4	853	494	0.02%	0.003%
41	6.751	1771	1776	1780	rBV7	782	894	0.04%	0.005%
42	6.796	1788	1790	1793	rBV2	379	186	0.01%	0.001%
43	6.825	1797	1799	1802	rVB2	753	366	0.01%	0.002%
44	6.905	1812	1824	1856	rBV	297015	582498	22.93%	3.125%
45	7.233	1915	1926	1958	rBV	1110429	1961225	77.21%	10.522%
46	7.545	2015	2023	2052	rBV	195742	369971	14.57%	1.985%
47	7.944	2144	2147	2151	rBV2	1297	958	0.04%	0.005%
48	7.973	2153	2156	2159	rVB2	627	383	0.02%	0.002%
49	8.021	2162	2171	2215	rBV2	300850	688499	27.11%	3.694%
50	8.619	2355	2357	2359	rBV4	550	257	0.01%	0.001%
51	8.651	2360	2367	2369	rBV7	1778	1967	0.08%	0.011%
52	8.735	2391	2393	2395	rBV3	649	355	0.01%	0.002%
53	8.776	2395	2406	2440	rBV	1201621	2001136	78.78%	10.736%
54	9.275	2557	2561	2563	rBV4	829	594	0.02%	0.003%
55	9.307	2569	2571	2574	rBV2	509	298	0.01%	0.002%
56	9.326	2574	2577	2582	rVB6	728	656	0.03%	0.004%
57	9.346	2582	2583	2585	rBV2	362	150	0.01%	0.001%
58	9.394	2595	2598	2600	rBV2	1108	607	0.02%	0.003%
59	9.416	2603	2605	2609	rVB3	679	434	0.02%	0.002%
60	9.436	2609	2611	2615	rVB2	941	495	0.02%	0.003%
61	9.465	2616	2620	2622	rBV4	592	478	0.02%	0.003%
62	9.522	2636	2638	2641	rVB2	565	258	0.01%	0.001%
63	9.558	2647	2649	2652	rBV2	798	376	0.01%	0.002%
64	9.625	2669	2670	2672	rBV2	364	203	0.01%	0.001%
65	9.645	2673	2676	2681	rVB5	946	857	0.03%	0.005%
66	9.667	2681	2683	2684	rBV2	230	102	0.00%	0.001%
67	9.683	2684	2688	2689	rBV4	705	450	0.02%	0.002%
68	9.841	2734	2737	2739	rBV2	581	275	0.01%	0.001%
69	9.886	2739	2751	2759	rBV8	5787	10053	0.40%	0.054%
70	9.937	2763	2767	2770	rBV5	1043	893	0.04%	0.005%
71	10.053	2800	2803	2806	rBV3	534	497	0.02%	0.003%
72	10.075	2808	2810	2812	rVB3	636	259	0.01%	0.001%
73	10.088	2812	2814	2816	rBV3	365	201	0.01%	0.001%
74	10.143	2817	2831	2850	rBV	674406	1057195	41.62%	5.672%
75	10.397	2909	2910	2915	rBV2	833	514	0.02%	0.003%
76	10.481	2927	2936	2938	rBV5	1298	1969	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
 Data File : VV037716.D
 Acq On : 02 Oct 2024 13:17
 Operator : SY/MD
 Sample : P4239-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.532	2949	2952	2954	rBV3	530	406	0.02%	0.002%
78	10.628	2976	2982	2983	rBV6	1983	1675	0.07%	0.009%
79	10.693	3000	3002	3005	rBV	426	259	0.01%	0.001%
80	10.712	3005	3008	3010	rVV2	524	272	0.01%	0.001%
81	10.747	3016	3019	3024	rVB3	956	615	0.02%	0.003%
82	10.786	3024	3031	3034	rBV6	1774	1987	0.08%	0.011%
83	10.937	3074	3078	3080	rBV3	784	751	0.03%	0.004%
84	10.995	3087	3096	3101	rBV7	1869	2543	0.10%	0.014%
85	11.124	3128	3136	3142	rBV7	9240	13877	0.55%	0.074%
86	11.178	3142	3153	3179	rBV	1167484	1861865	73.30%	9.989%
87	11.551	3258	3269	3306	rVB	1199972	1911905	75.27%	10.258%
88	12.741	3637	3639	3642	rBV2	924	518	0.02%	0.003%
89	12.773	3646	3649	3653	rBV3	635	478	0.02%	0.003%
90	12.796	3653	3656	3657	rVB	440	237	0.01%	0.001%
91	12.844	3668	3671	3673	rBV3	1076	686	0.03%	0.004%
92	12.857	3673	3675	3679	rVV2	664	348	0.01%	0.002%
93	13.008	3716	3722	3723	rBV2	778	650	0.03%	0.003%
94	13.027	3726	3728	3732	rVB2	681	425	0.02%	0.002%
95	13.085	3744	3746	3748	rBV2	673	389	0.02%	0.002%
96	13.181	3773	3776	3778	rBV2	822	585	0.02%	0.003%
97	13.198	3778	3781	3782	rBV2	1128	643	0.03%	0.003%
98	13.365	3831	3833	3837	rBV4	693	408	0.02%	0.002%
99	14.008	4031	4033	4035	rBV2	598	266	0.01%	0.001%
100	14.114	4061	4066	4070	rBV2	1098	1218	0.05%	0.007%


Sum of corrected areas: 18638845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037716.D
Acq On : 02 Oct 2024 13:17
Operator : SY/MD
Sample : P4239-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

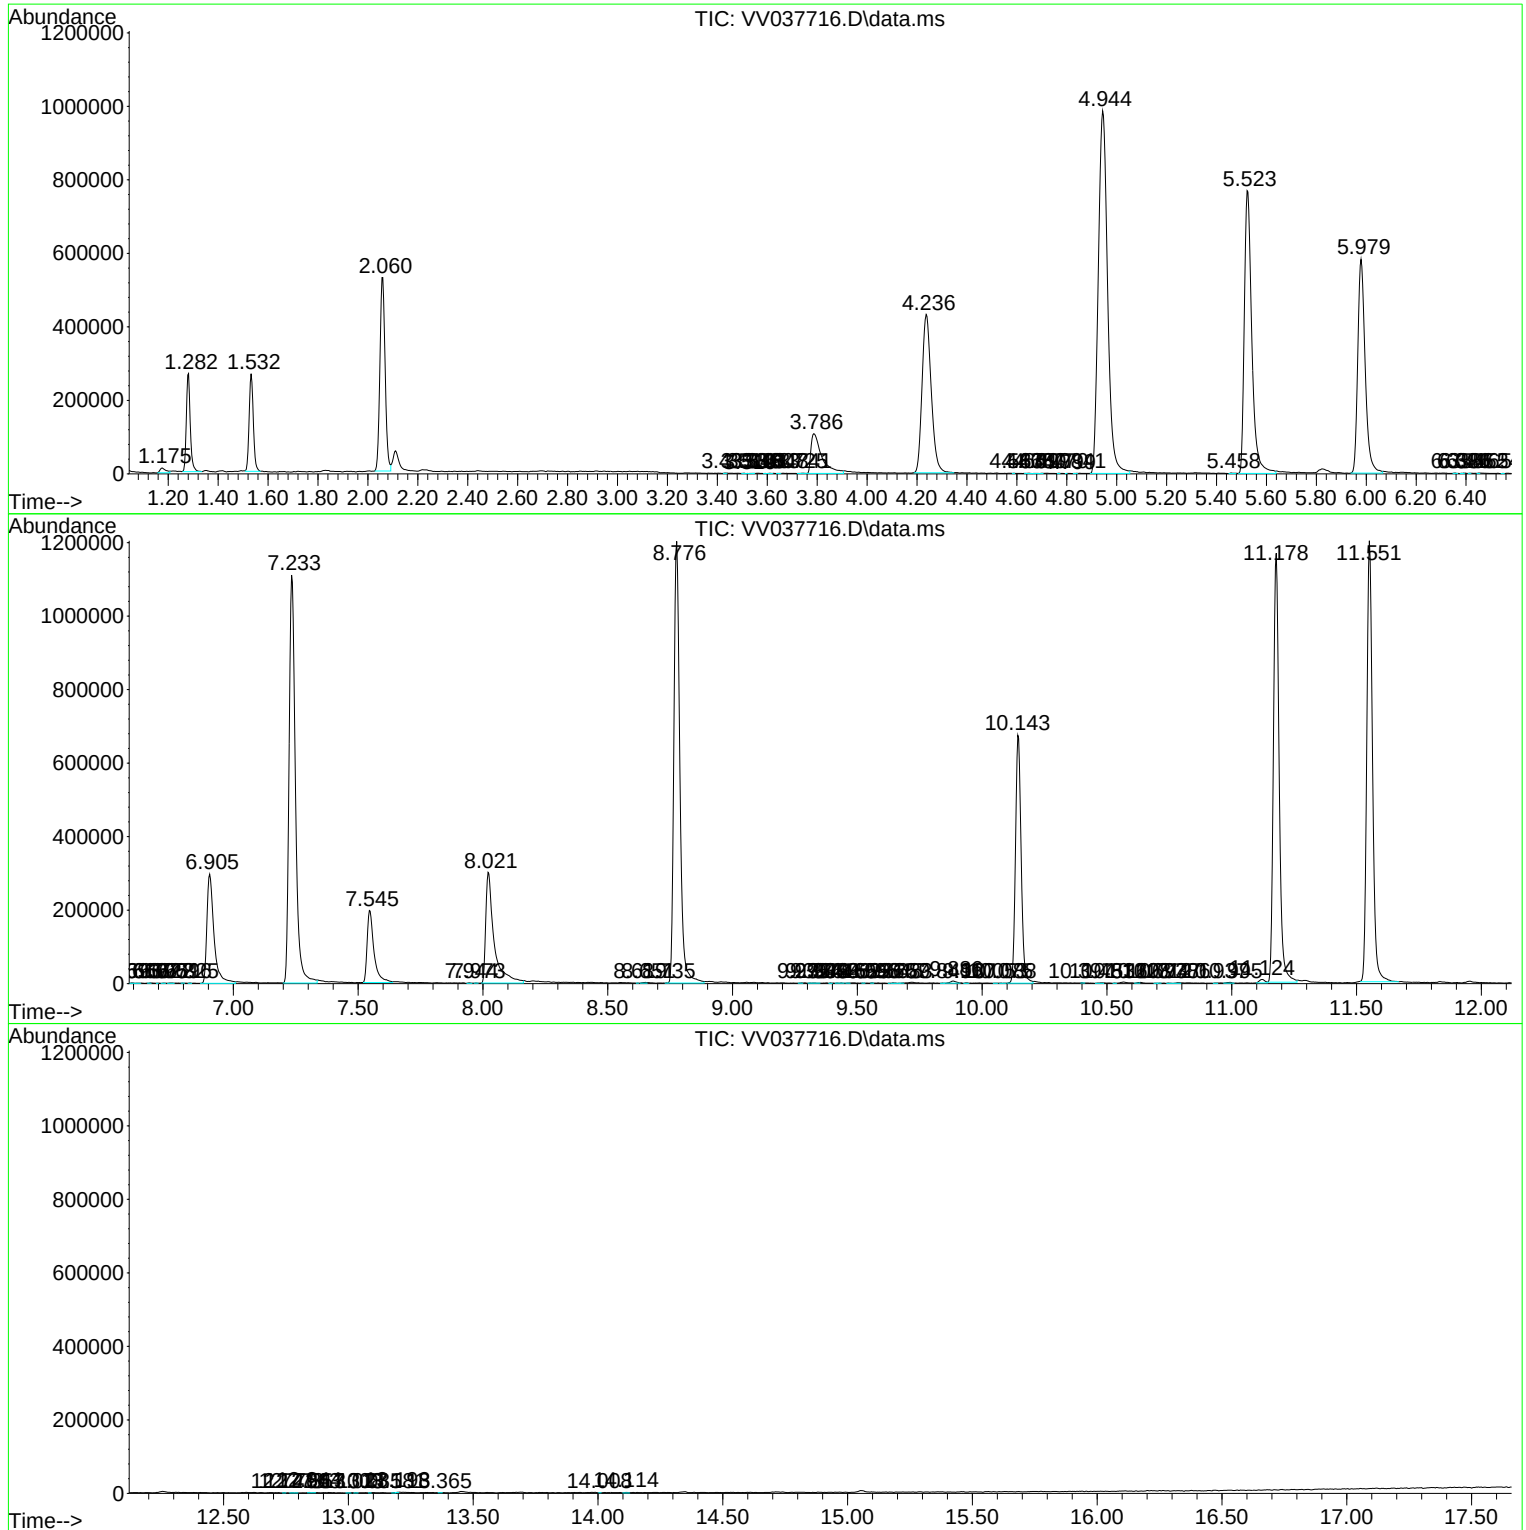

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037716.D
Acq On : 02 Oct 2024 13:17
Operator : SY/MD
Sample : P4239-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037716.D
Acq On : 02 Oct 2024 13:17
Operator : SY/MD
Sample : P4239-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------