
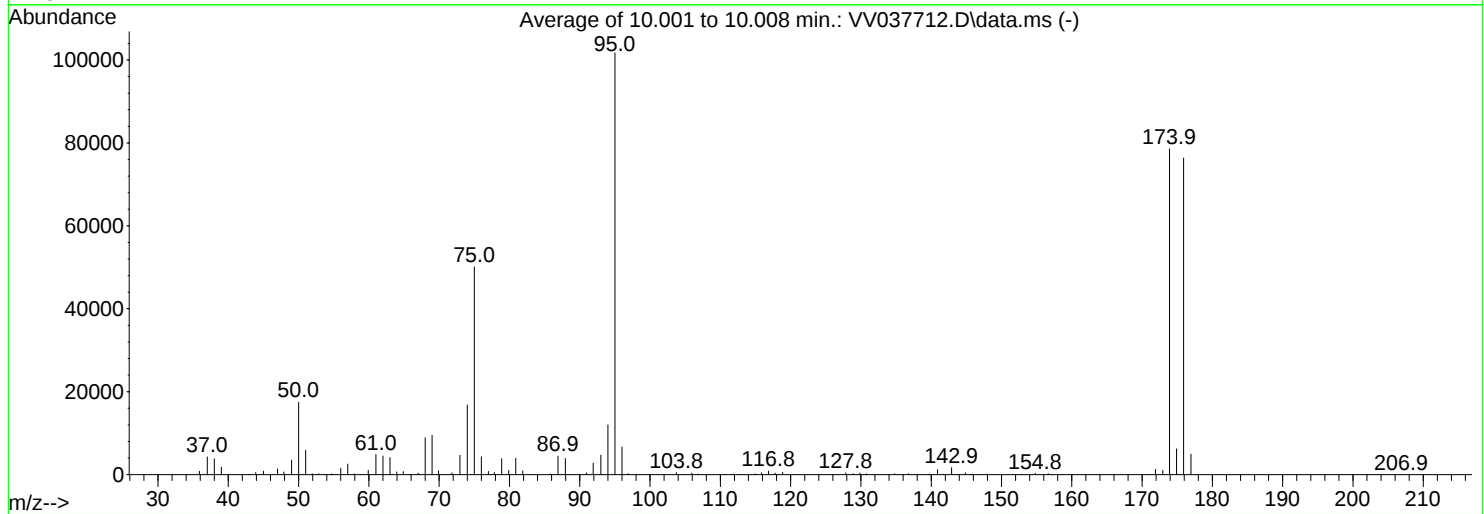


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100224\
Data File : VV037712.D
Acq On : 02 Oct 2024 08:17
Operator : SY/MD
Sample : BFB385
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB385

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Thu Oct 03 05:55:19 2024

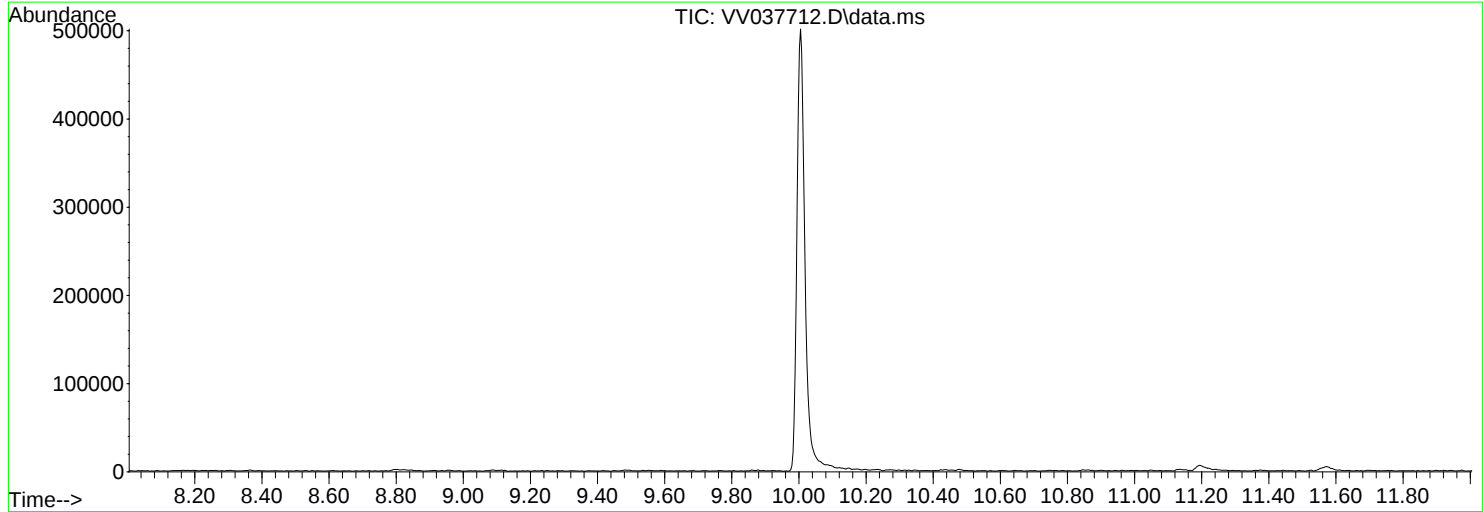

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	17443	PASS
75	95	30	80	49.2	50067	PASS
95	95	100	100	100.0	101715	PASS
96	95	5	9	6.5	6650	PASS
173	174	0.00	2	1.3	1060	PASS
174	95	50	120	77.2	78571	PASS
175	174	5	9	7.9	6229	PASS
176	174	95	105	97.2	76365	PASS
177	176	5	10	6.5	4931	PASS

m/z	Abundance
39.90	323.0
43.90	483.0

Instrument :
MSVOA_V
ClientSampleId :
BFB385

m/z	Abundance
35.90	865.0
37.00	4332.0
38.00	3968.0
39.00	1889.0
39.90	263.0
42.90	121.0
43.90	959.0
45.00	919.0
47.00	1278.0
47.90	658.0
49.00	3623.0
50.00	17240.0
51.00	5743.0
51.90	263.0
52.80	207.0
53.70	108.0
54.70	319.0
56.00	1534.0
57.00	2482.0
57.90	184.0
59.90	1011.0
61.00	4957.0
62.00	4518.0
63.00	4336.0
64.00	642.0
64.90	727.0
66.00	125.0
67.00	366.0
68.00	8591.0
69.00	9916.0
69.90	935.0
71.80	417.0
73.00	4709.0
74.00	16784.0
75.00	50488.0
76.00	4364.0
77.00	722.0
77.90	504.0
78.90	3982.0
79.90	980.0
80.90	3825.0
81.90	937.0
85.80	199.0
86.90	4378.0
88.00	3830.0
90.90	443.0
91.90	2667.0
93.00	4807.0
94.00	11843.0
95.00	100680.0
96.00	6887.0
96.90	237.0
103.80	477.0
104.70	162.0
105.90	379.0
106.80	132.0
112.00	135.0
114.90	163.0
115.80	408.0
116.80	913.0
117.80	426.0
118.80	599.0
127.90	429.0
129.00	238.0
129.80	347.0
130.80	169.0
134.80	202.0
136.80	223.0
139.70	172.0
140.90	1136.0
141.70	178.0
142.90	1430.0
143.80	108.0
144.90	491.0
145.80	127.0
148.00	179.0
152.90	115.0
154.80	205.0
156.60	183.0
157.10	135.0
171.90	1140.0
173.00	1026.0
173.90	76472.0
174.90	6264.0
175.90	74304.0
176.90	4750.0
206.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB385

m/z	Abundance
35.90	835.0
37.00	4468.0
38.00	3933.0
39.00	1877.0
39.90	279.0
42.00	119.0
43.90	991.0
45.00	885.0
47.00	1460.0
47.90	701.0
49.00	3563.0
50.00	18120.0
51.00	6082.0
52.00	261.0
52.90	185.0
54.70	255.0
56.00	1617.0
57.00	2639.0
57.90	186.0
59.90	1090.0
61.00	5046.0
62.00	4583.0
63.00	4260.0
63.90	657.0
64.90	752.0
67.00	346.0
68.00	9188.0
69.00	9812.0
69.90	946.0
71.80	430.0
73.00	4902.0
74.00	17288.0
75.00	51616.0
76.00	4376.0
77.00	824.0
77.90	551.0
78.90	4004.0
79.90	1035.0
80.90	4060.0
81.90	898.0
85.80	177.0
86.90	4577.0
88.00	3944.0
88.70	112.0
90.90	463.0
91.90	2890.0
93.00	4805.0
94.00	12341.0
95.00	105016.0
96.00	6791.0
96.90	240.0
103.80	525.0
104.80	129.0
105.90	380.0
106.80	160.0
111.90	143.0
112.70	109.0
114.90	223.0
115.90	468.0
116.80	871.0
117.80	396.0
118.80	574.0
127.90	450.0
128.90	263.0
129.80	461.0
130.80	199.0
134.80	184.0
136.80	250.0
139.70	197.0
140.90	1247.0
141.70	158.0
142.90	1782.0
144.80	471.0
145.80	130.0
147.90	165.0
152.90	102.0
154.80	316.0
156.70	271.0
157.10	156.0
171.90	1321.0
172.90	1094.0
173.90	81392.0
174.90	6513.0
175.90	79200.0
177.00	5123.0
177.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB385

m/z	Abundance
35.90	766.0
37.00	4109.0
38.00	3608.0
39.00	1714.0
39.90	301.0
42.10	133.0
44.00	1000.0
45.00	729.0
47.00	1432.0
47.90	651.0
49.00	3343.0
50.00	16968.0
51.00	5887.0
52.00	235.0
52.90	154.0
54.90	228.0
56.00	1521.0
57.00	2572.0
57.90	174.0
59.90	1079.0
61.00	4626.0
62.00	4386.0
63.00	3827.0
63.90	645.0
64.90	765.0
67.00	300.0
68.00	8990.0
69.00	8762.0
69.90	863.0
71.80	448.0
72.90	4381.0
74.00	16288.0
75.00	48096.0
76.00	4211.0
77.00	808.0
77.80	539.0
78.90	3647.0
79.90	949.0
80.90	3970.0
81.90	874.0
85.80	128.0
86.90	4457.0
87.90	3933.0
91.00	428.0
91.90	2806.0
93.00	4509.0
94.00	11849.0
95.00	99448.0
96.00	6273.0
96.90	263.0
103.70	481.0
106.00	356.0
106.90	165.0
110.70	112.0
111.80	165.0
112.70	147.0
115.00	200.0
115.90	502.0
116.90	728.0
117.80	351.0
118.90	526.0
127.80	449.0
128.80	239.0
129.90	472.0
130.80	180.0
134.80	163.0
136.80	250.0
139.80	134.0
140.90	1223.0
142.90	1854.0
144.80	448.0
145.80	118.0
147.90	143.0
154.80	371.0
156.70	362.0
158.70	117.0
170.70	203.0
171.90	1343.0
172.90	1059.0
173.90	77848.0
174.90	5911.0
175.90	75592.0
177.00	4919.0
177.80	122.0
206.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB385