

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
 Data File : VV028276.D
 Acq On : 03 Oct 2022 13:56
 Operator : SY/MD
 Sample : N4865-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 04 02:43:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound			R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards								
1) 1,4-Difluorobenzene			5.613	114	186956	5.000	ug/L	0.00
28) Chlorobenzene-d5			8.847	117	188418	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4			11.246	152	84658	5.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3			1.301	65	71729	5.106	ug/L	0.00
Spiked Amount 5.000			Range 40 - 130		Recovery	= 102.200%		
7) Chloroethane-d5			1.561	69	65239	5.486	ug/L	0.00
Spiked Amount 5.000			Range 65 - 130		Recovery	= 109.800%		
11) 1,1-Dichloroethene-d2			2.098	63	103055	3.892	ug/L	0.00
Spiked Amount 5.000			Range 60 - 125		Recovery	= 77.800%		
20) 2-Butanone-d5			3.896	46	97154	40.876	ug/L	0.00
Spiked Amount 50.000			Range 40 - 130		Recovery	= 81.760%		
24) Chloroform-d			4.339	84	130808	5.140	ug/L	0.00
Spiked Amount 5.000			Range 70 - 125		Recovery	= 102.800%		
26) 1,2-Dichloroethane-d4			5.024	65	63409	5.375	ug/L	0.00
Spiked Amount 5.000			Range 70 - 130		Recovery	= 107.400%		
32) Benzene-d6			5.040	84	276608	5.352	ug/L	0.00
Spiked Amount 5.000			Range 70 - 125		Recovery	= 107.000%		
36) 1,2-Dichloropropane-d6			6.063	67	81600	5.503	ug/L	0.00
Spiked Amount 5.000			Range 60 - 140		Recovery	= 110.000%		
41) Toluene-d8			7.310	98	233254	4.907	ug/L	0.00
Spiked Amount 5.000			Range 70 - 130		Recovery	= 98.200%		
43) trans-1,3-Dichloroprop...			7.622	79	27140	4.806	ug/L	0.00
Spiked Amount 5.000			Range 55 - 130		Recovery	= 96.200%		
46) 2-Hexanone-d5			8.088	63	114892	49.706	ug/L	0.00
Spiked Amount 50.000			Range 45 - 130		Recovery	= 99.420%		
56) 1,1,2,2-Tetrachloroeth...			10.214	84	58676	5.221	ug/L	0.00
Spiked Amount 5.000			Range 65 - 120		Recovery	= 104.400%		
66) 1,2-Dichlorobenzene-d4			11.622	152	82173	5.640	ug/L	0.00
Spiked Amount 5.000			Range 80 - 120		Recovery	= 112.800%		
Target Compounds								Qvalue
16) Methylene chloride			2.500	84	5095	0.338	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028276.D
Acq On : 03 Oct 2022 13:56
Operator : SY/MD
Sample : N4865-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 04 02:43:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

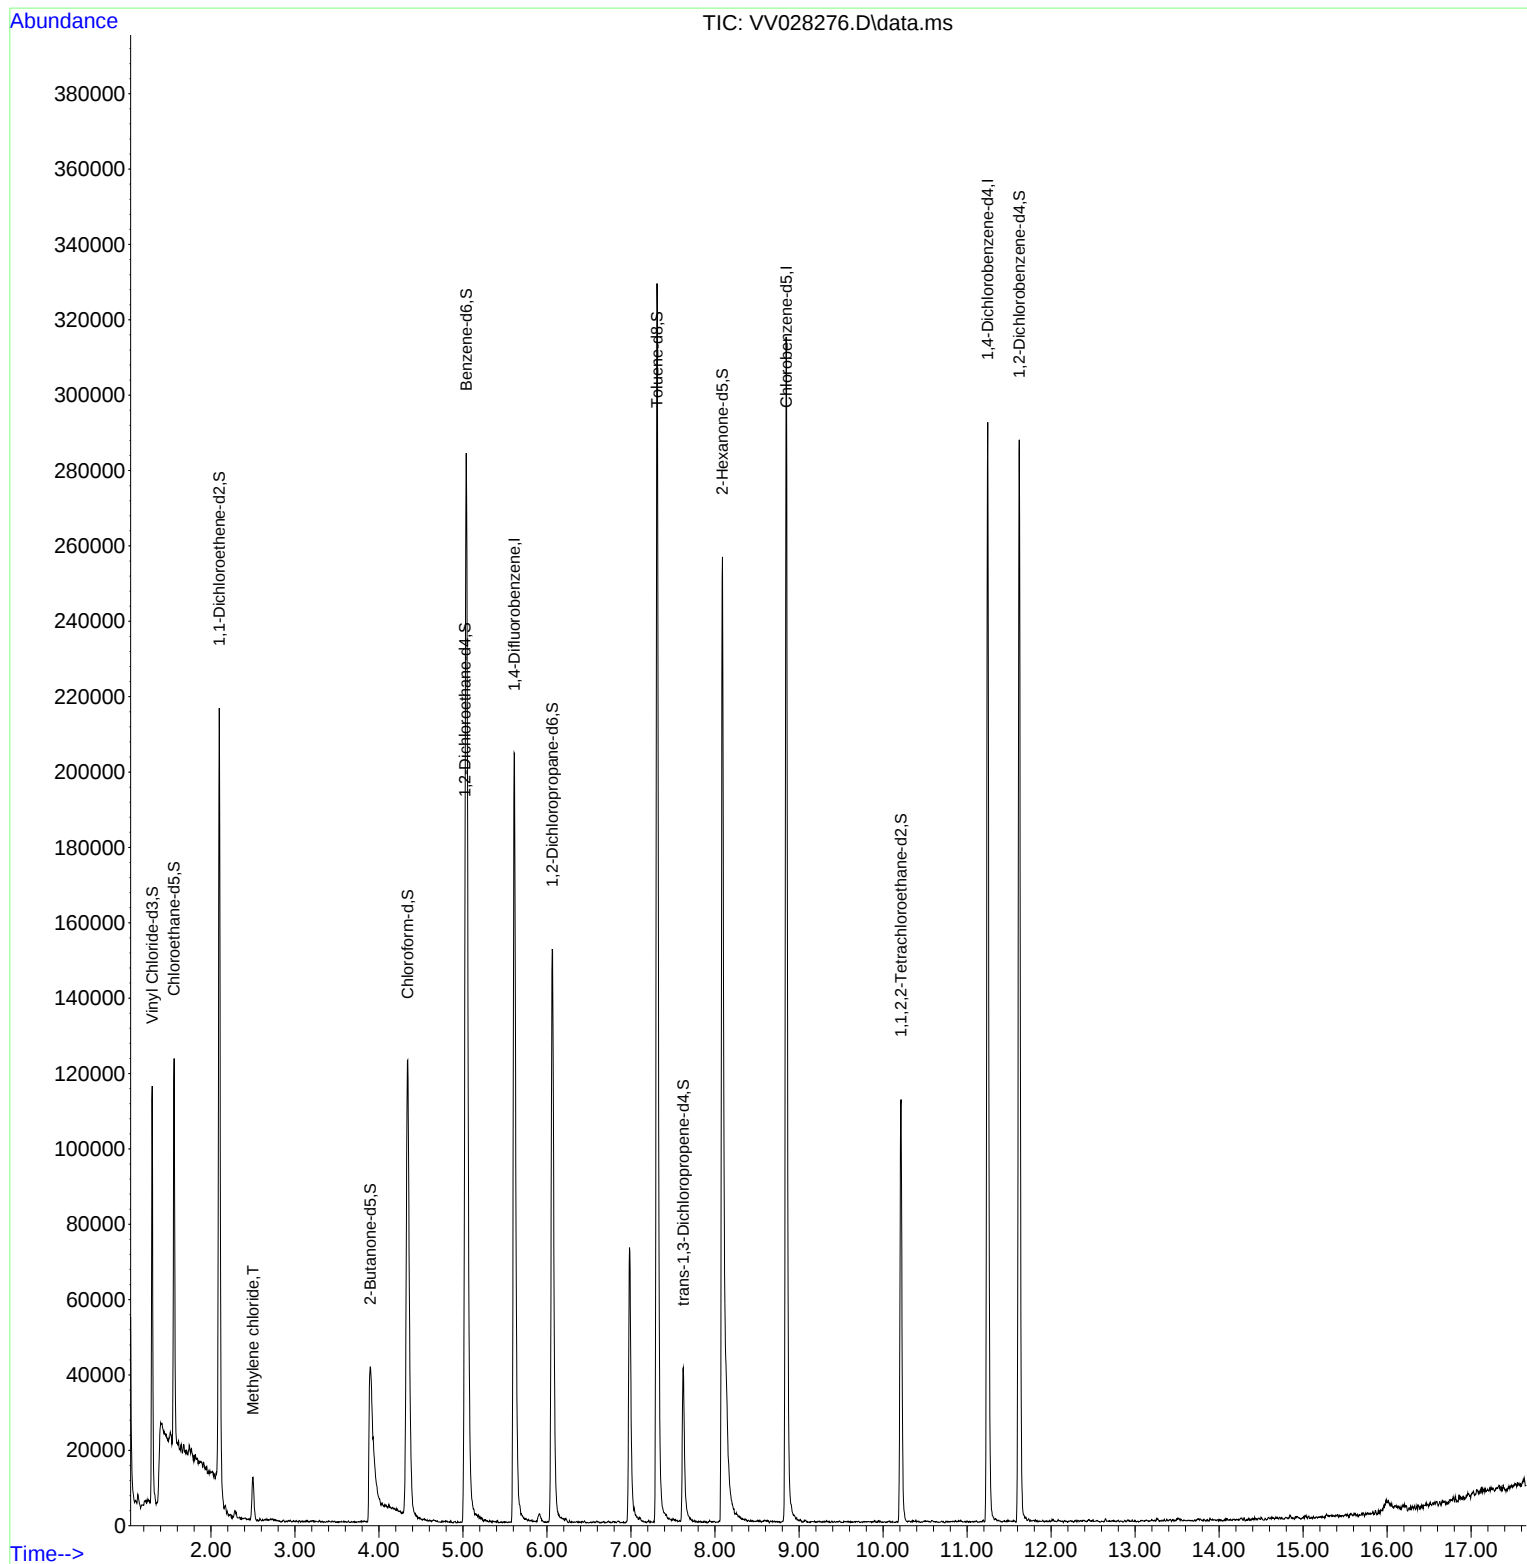

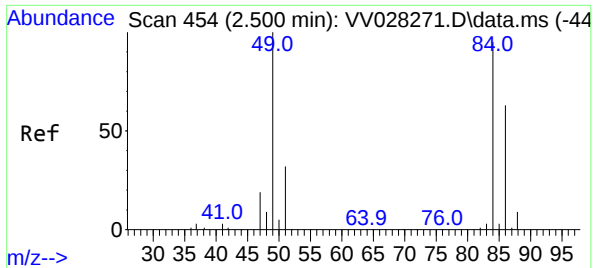

#16
Methylene chloride
Concen: 0.338 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028276.D
Acq: 03 Oct 2022 13:56

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 5095
Ion Ratio Lower Upper
84 100
86 59.1 46.8 86.8
49 100.4 87.5 162.5

