

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100322\
 Data File : VW028284.D
 Acq On : 03 Oct 2022 17:35
 Operator : SY/MD
 Sample : N4870-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 04 02:46:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	195654	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	195835	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	89530	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	72410	4.925	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.600%
7) Chloroethane-d5	1.561	69	63243	5.082	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.600%
11) 1,1-Dichloroethene-d2	2.101	63	107544	3.881	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%
20) 2-Butanone-d5	3.902	46	140845	56.624	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.240%
24) Chloroform-d	4.339	84	145269	5.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.000%
26) 1,2-Dichloroethane-d4	5.027	65	68261	5.529	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.600%
32) Benzene-d6	5.043	84	289397	5.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.800%
36) 1,2-Dichloropropane-d6	6.066	67	86964	5.643	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.800%
41) Toluene-d8	7.313	98	242933	4.917	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	7.622	79	23241	3.960	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.088	63	124246	51.718	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.440%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	61471	5.262	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	85552	5.552	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.000%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	4409	0.279	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028284.D
Acq On : 03 Oct 2022 17:35
Operator : SY/MD
Sample : N4870-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 04 02:46:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

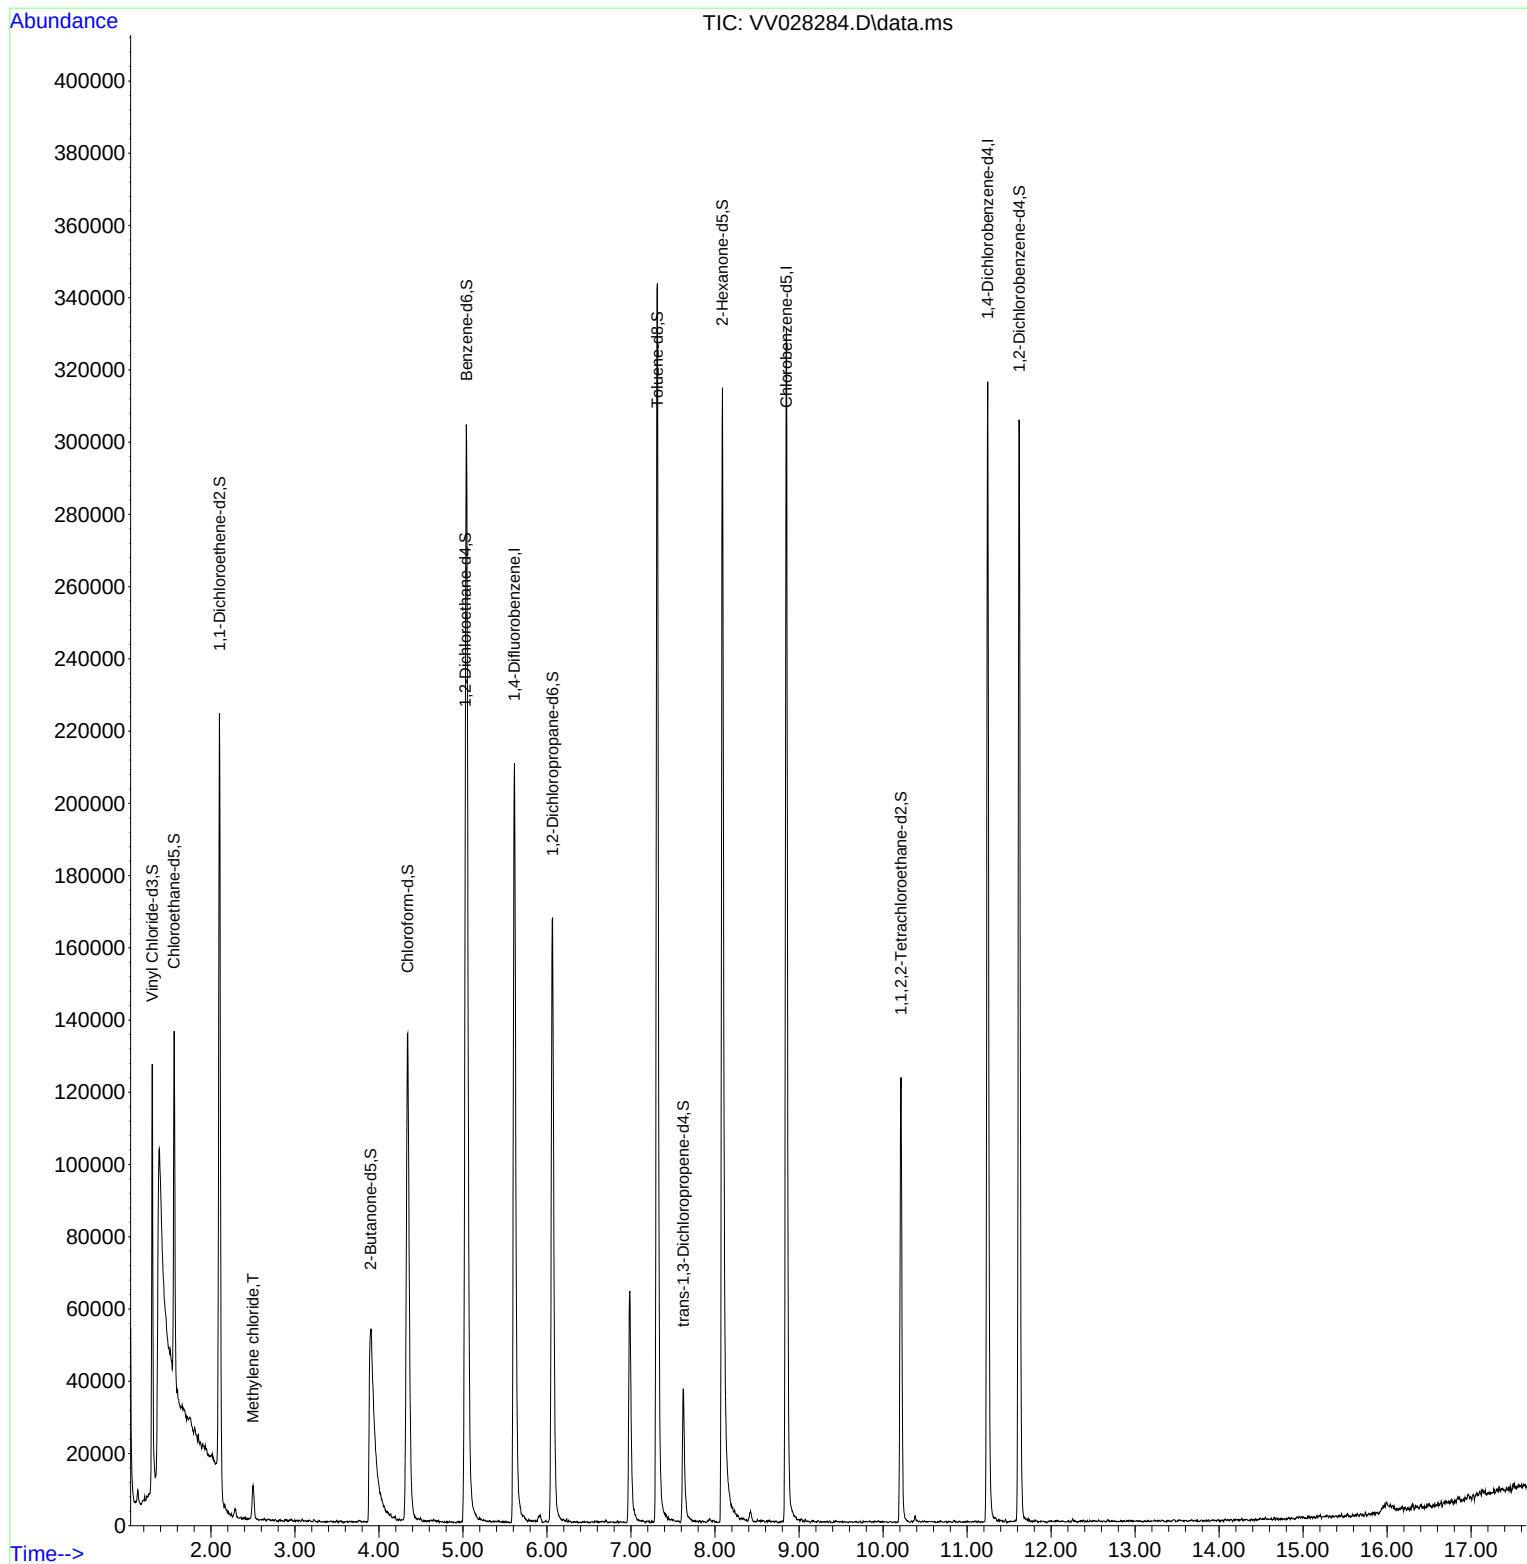

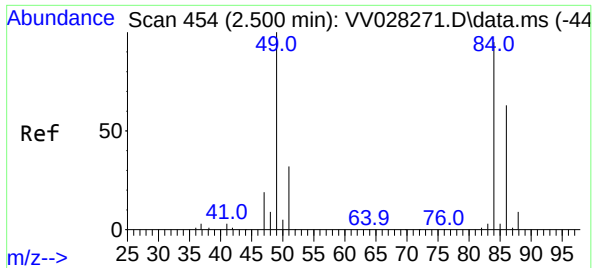

#16
Methylene chloride
Concen: 0.279 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028284.D
Acq: 03 Oct 2022 17:35

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4409
Ion Ratio Lower Upper
84 100
86 62.5 46.8 86.8
49 106.7 87.5 162.5

