

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
 Data File : VV028285.D
 Acq On : 03 Oct 2022 17:59
 Operator : SY/MD
 Sample : N4730-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 04 02:46:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	180936	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	184517	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	84314	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	72151	5.307	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.200%
7) Chloroethane-d5	1.561	69	64863	5.636	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.800%
11) 1,1-Dichloroethene-d2	2.101	63	105953	4.135	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	3.899	46	147883	64.290	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.580%
24) Chloroform-d	4.339	84	141944	5.763	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.200%
26) 1,2-Dichloroethane-d4	5.027	65	66293	5.806	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.200%
32) Benzene-d6	5.043	84	287650	5.683	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.600%
36) 1,2-Dichloropropane-d6	6.063	67	87298	6.012	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	120.200%
41) Toluene-d8	7.313	98	241193	5.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
43) trans-1,3-Dichloroprop...	7.622	79	24419	4.416	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.400%
46) 2-Hexanone-d5	8.088	63	126051	55.687	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.380%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	62196	5.651	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	86505	5.962	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.200%
Target Compounds						
16) Methylene chloride	2.503	84	3964	0.271	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028285.D
Acq On : 03 Oct 2022 17:59
Operator : SY/MD
Sample : N4730-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 04 02:46:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

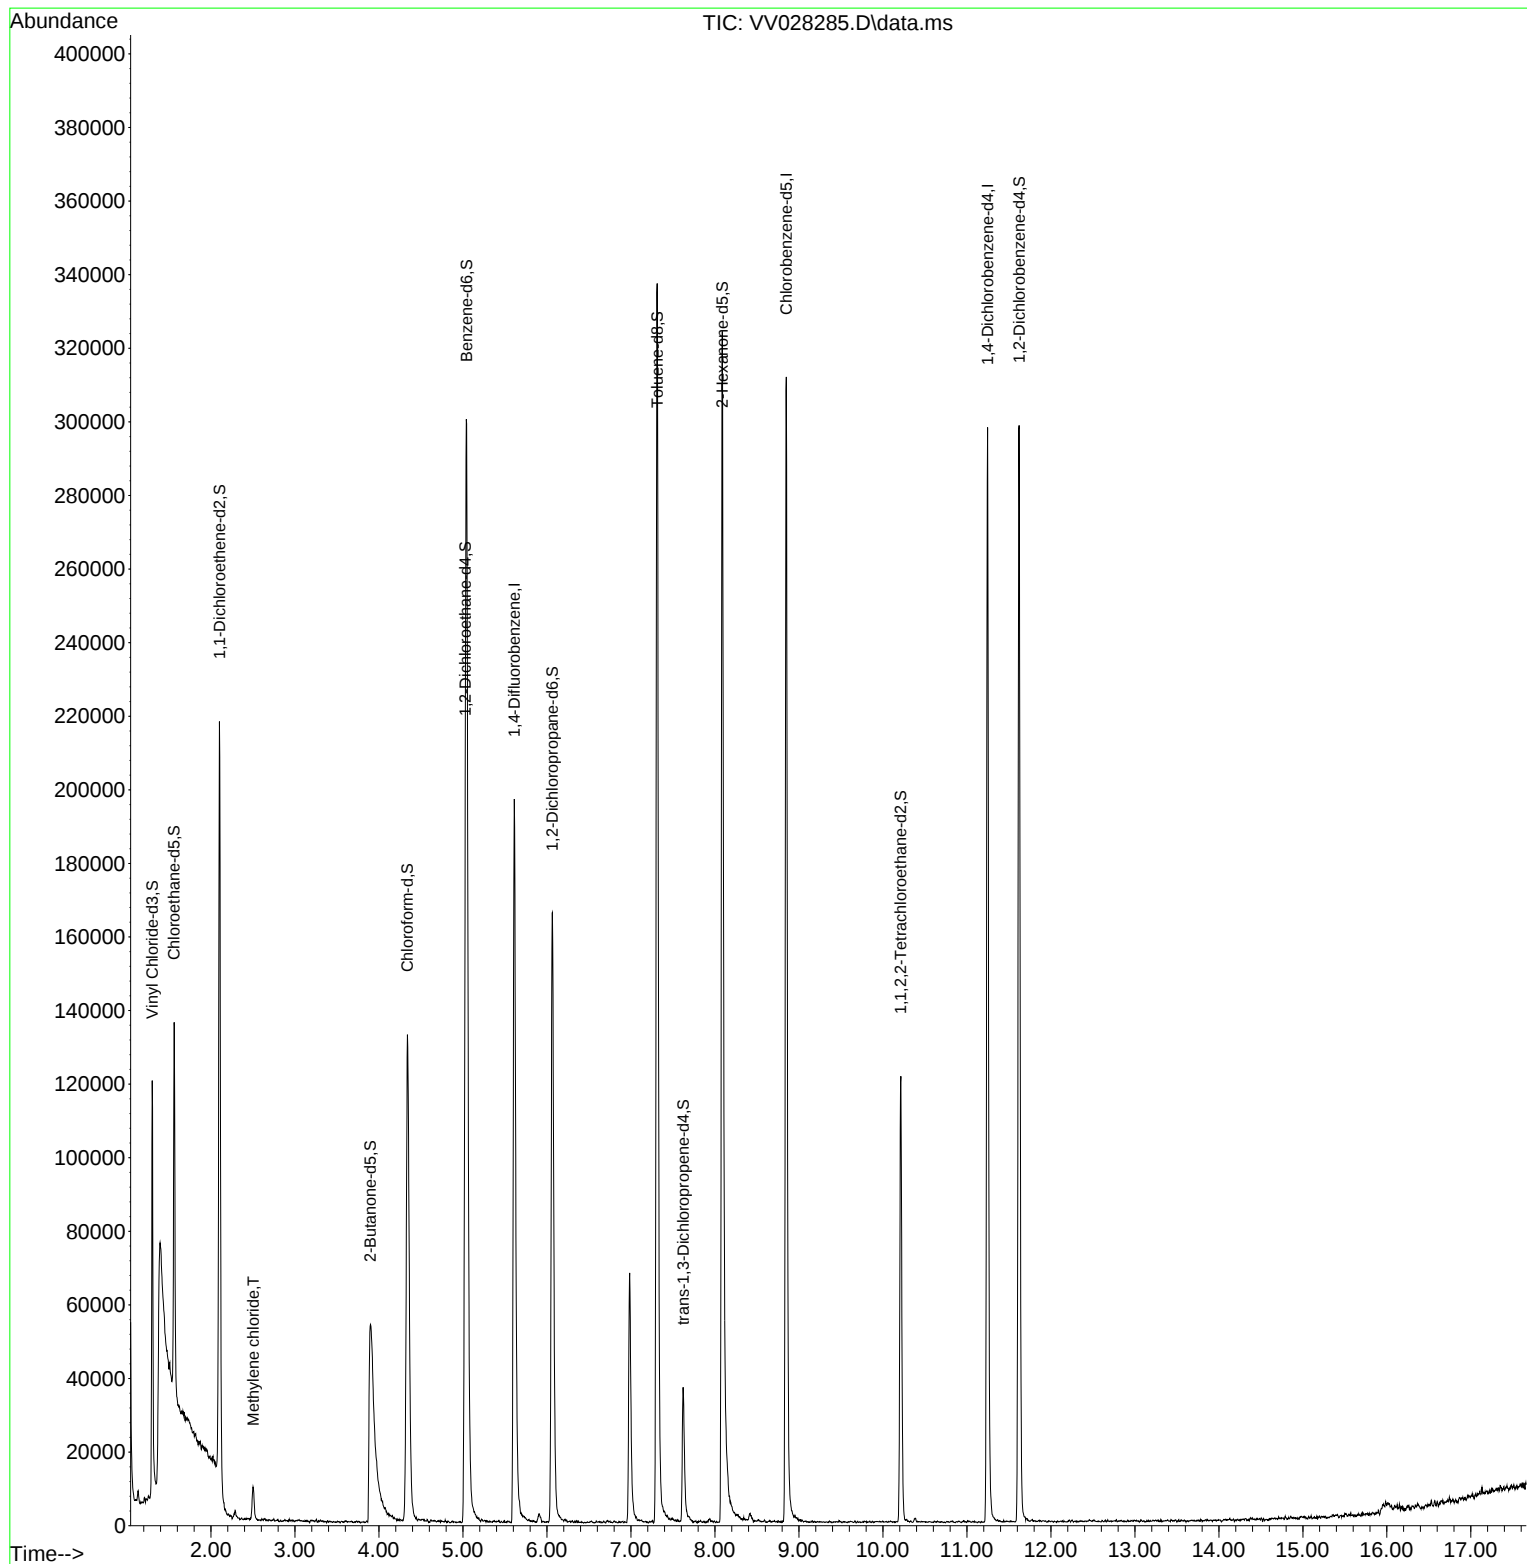

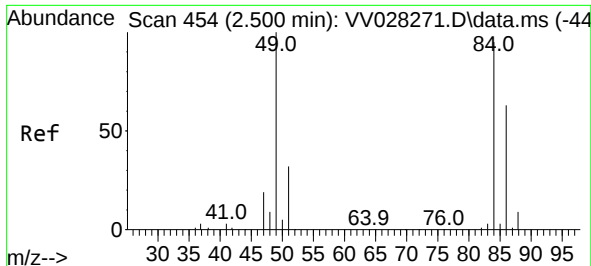

#16
Methylene chloride
Concen: 0.271 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV028285.D
Acq: 03 Oct 2022 17:59

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 3964
Ion Ratio Lower Upper
84 100
86 64.7 46.8 86.8
49 101.3 87.5 162.5

