

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
 Data File : VV028294.D
 Acq On : 03 Oct 2022 21:38
 Operator : SY/MD
 Sample : N4856-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 04 06:16:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.613	114	196895	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.850	117	197426	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.246	152	91722	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.301	65	78052	5.276	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.600%	
7) Chloroethane-d5		1.561	69	65919	5.263	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.200%	
11) 1,1-Dichloroethene-d2		2.102	63	109467	3.926	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.600%	
20) 2-Butanone-d5		3.896	46	145208	58.010	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.020%	
24) Chloroform-d		4.339	84	140907	5.257	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%	
26) 1,2-Dichloroethane-d4		5.027	65	69519	5.595	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.800%	
32) Benzene-d6		5.043	84	298310	5.508	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.200%	
36) 1,2-Dichloropropane-d6		6.066	67	88832	5.718	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.400%	
41) Toluene-d8		7.310	98	245971	4.938	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.800%	
43) trans-1,3-Dichloroprop...		7.622	79	26266	4.439	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%	
46) 2-Hexanone-d5		8.085	63	127159	52.504	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.000%	
56) 1,1,2,2-Tetrachloroeth...		10.214	84	63319	5.377	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4		11.622	152	89679	5.681	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.600%	
Target Compounds							
16) Methylene chloride		2.500	84	7627	0.480	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028294.D
Acq On : 03 Oct 2022 21:38
Operator : SY/MD
Sample : N4856-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 04 06:16:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

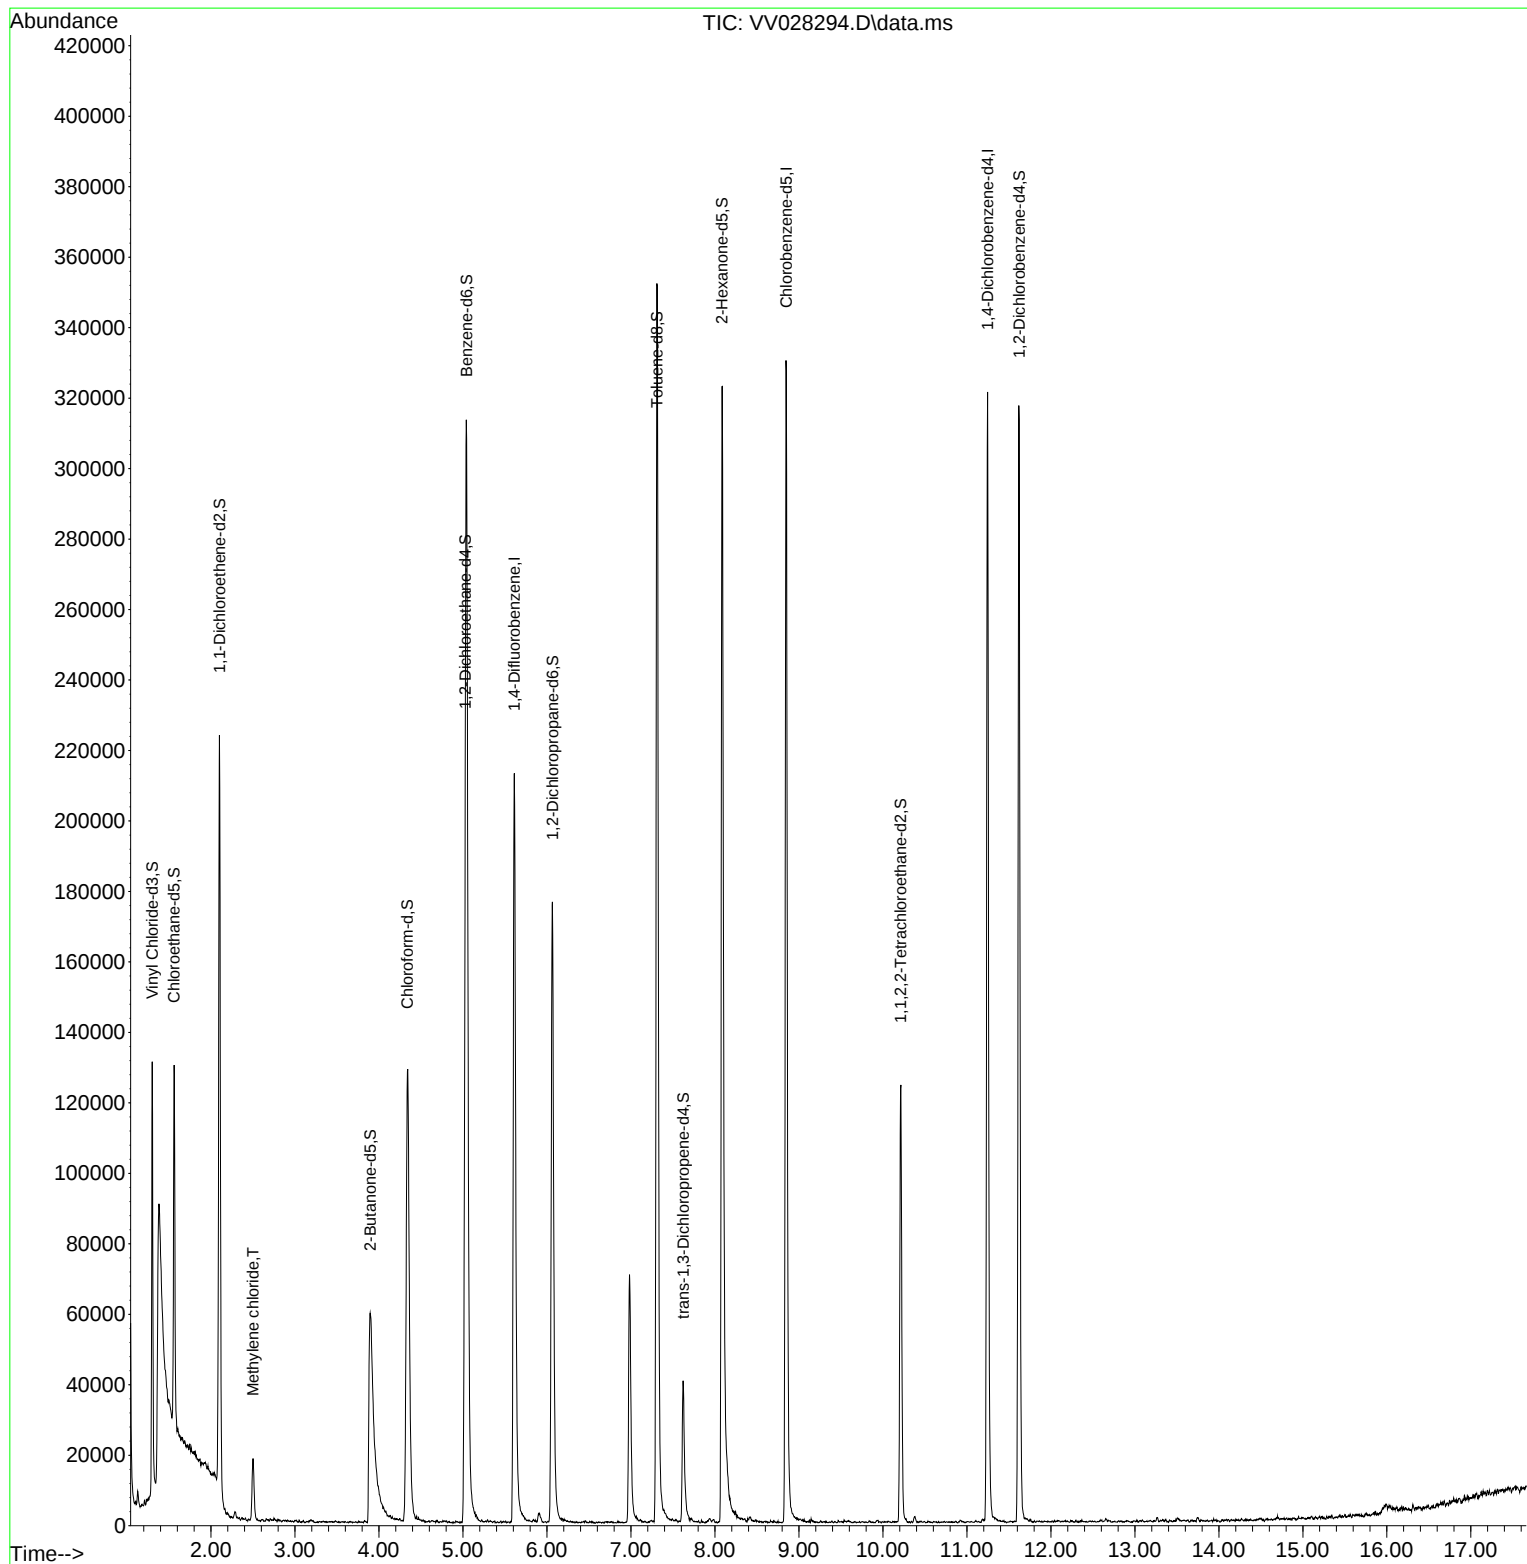

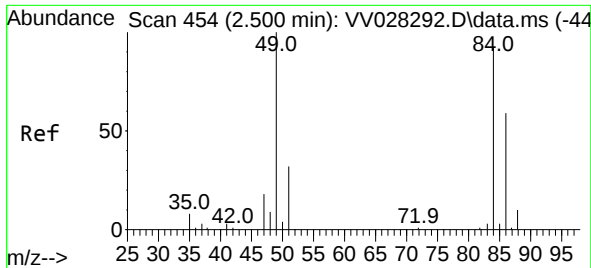

#16
Methylene chloride
Concen: 0.480 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028294.D
Acq: 03 Oct 2022 21:38

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 7627
Ion Ratio Lower Upper
84 100
86 61.6 46.8 86.8
49 105.9 87.5 162.5

