

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
 Data File : VV028307.D
 Acq On : 04 Oct 2022 02:53
 Operator : SY/MD
 Sample : N4866-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFR4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	98	rBV	6742536	7192480	100.00%	49.510%
2	1.561	156	162	176	rVB	98861	122471	1.70%	0.843%
3	2.101	321	330	348	rVB	204920	311454	4.33%	2.144%
4	3.902	873	890	932	rBV	731289	1893322	26.32%	13.033%
5	4.342	1008	1027	1054	rBV	127305	327065	4.55%	2.251%
6	5.040	1227	1244	1279	rBV2	299904	772349	10.74%	5.316%
7	5.612	1409	1422	1447	rBV	202363	416683	5.79%	2.868%
8	6.066	1543	1563	1589	rBV	167137	354378	4.93%	2.439%
9	6.985	1837	1849	1878	rBV	68604	135892	1.89%	0.935%
10	7.310	1938	1950	1973	rBV	325198	591468	8.22%	4.071%
11	7.622	2035	2047	2067	rBV	41480	78051	1.09%	0.537%
12	8.088	2179	2192	2221	rBV	307984	620870	8.63%	4.274%
13	8.850	2416	2429	2450	rBV	320514	527251	7.33%	3.629%
14	10.213	2841	2853	2869	rBV	126702	200825	2.79%	1.382%
15	11.246	3162	3174	3191	rBV	315110	484149	6.73%	3.333%
16	11.619	3279	3290	3307	rBV	319038	498711	6.93%	3.433%




Sum of corrected areas: 14527419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028307.D
Acq On : 04 Oct 2022 02:53
Operator : SY/MD
Sample : N4866-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

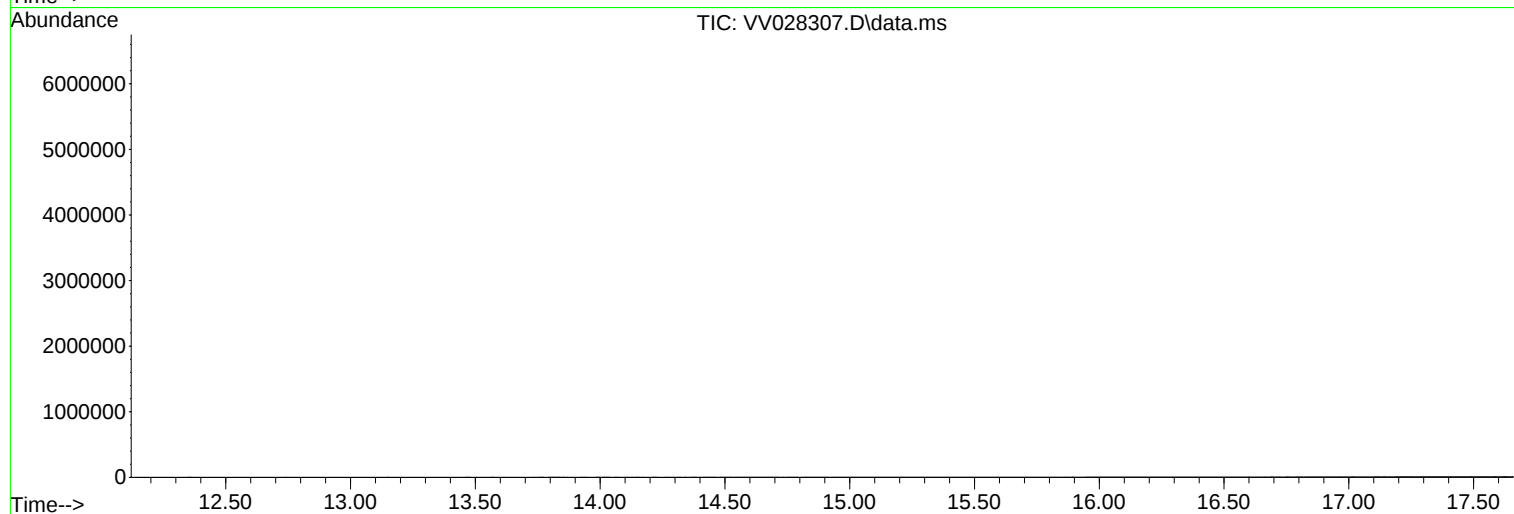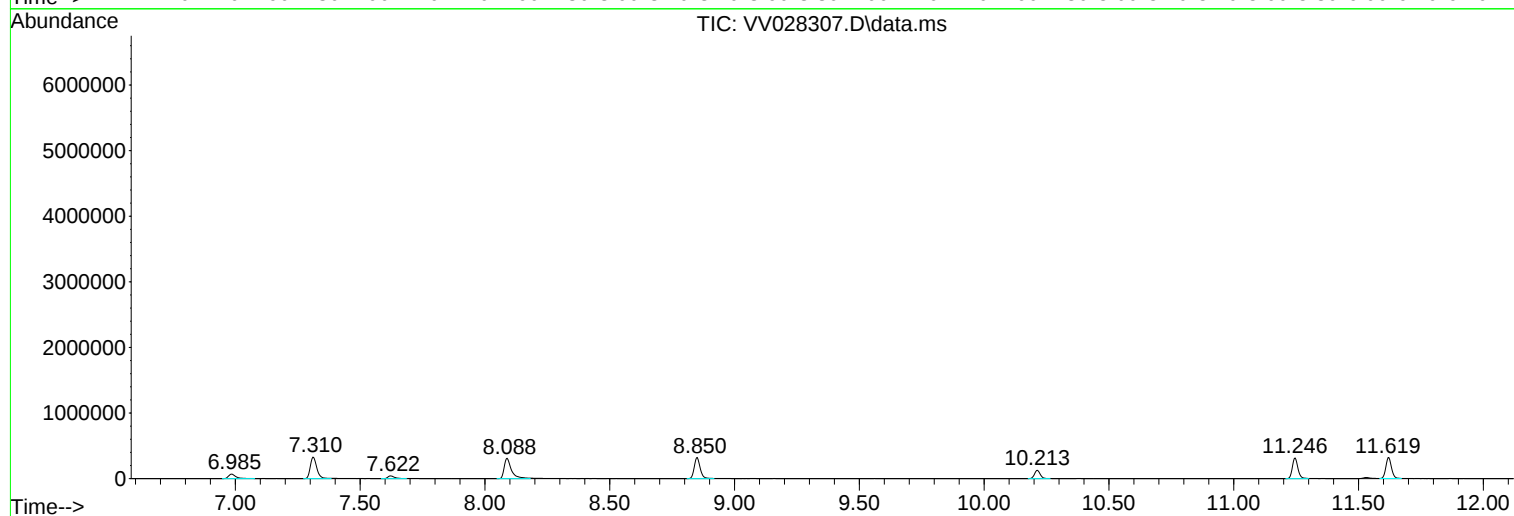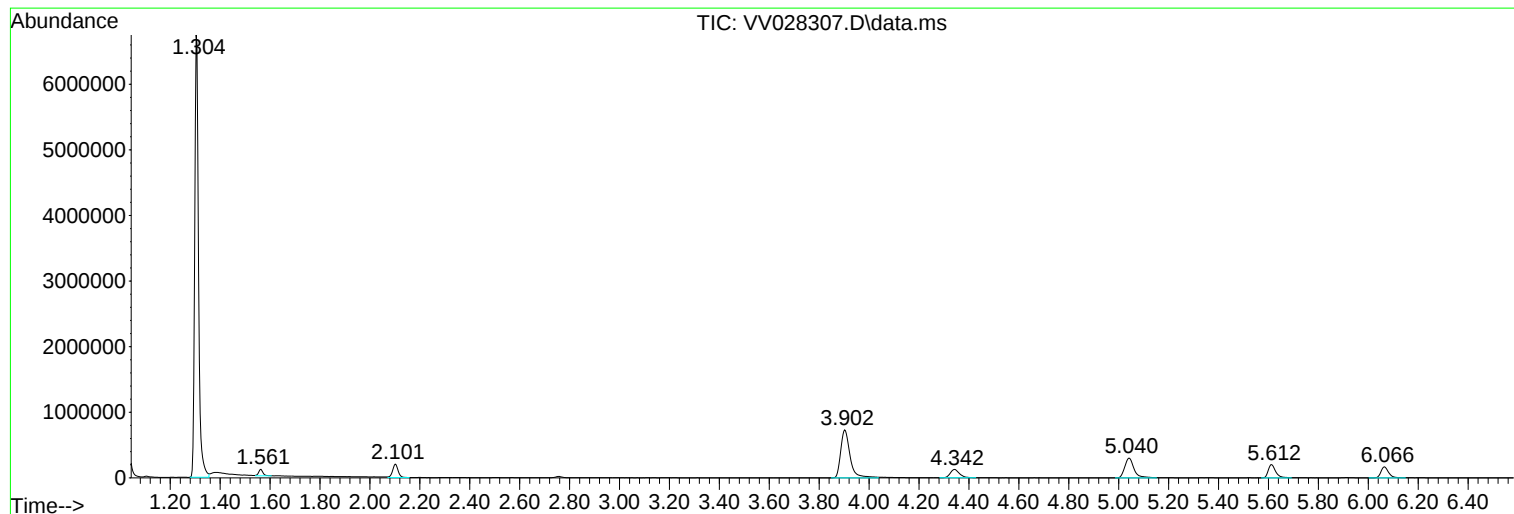

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028307.D
Acq On : 04 Oct 2022 02:53
Operator : SY/MD
Sample : N4866-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
Data File : VV028307.D
Acq On : 04 Oct 2022 02:53
Operator : SY/MD
Sample : N4866-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc