


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100322\
 Data File : VV028267.D
 Acq On : 03 Oct 2022 09:03
 Operator : SY/MD
 Sample : BFB381
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB381

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 04 02:28:45 2022

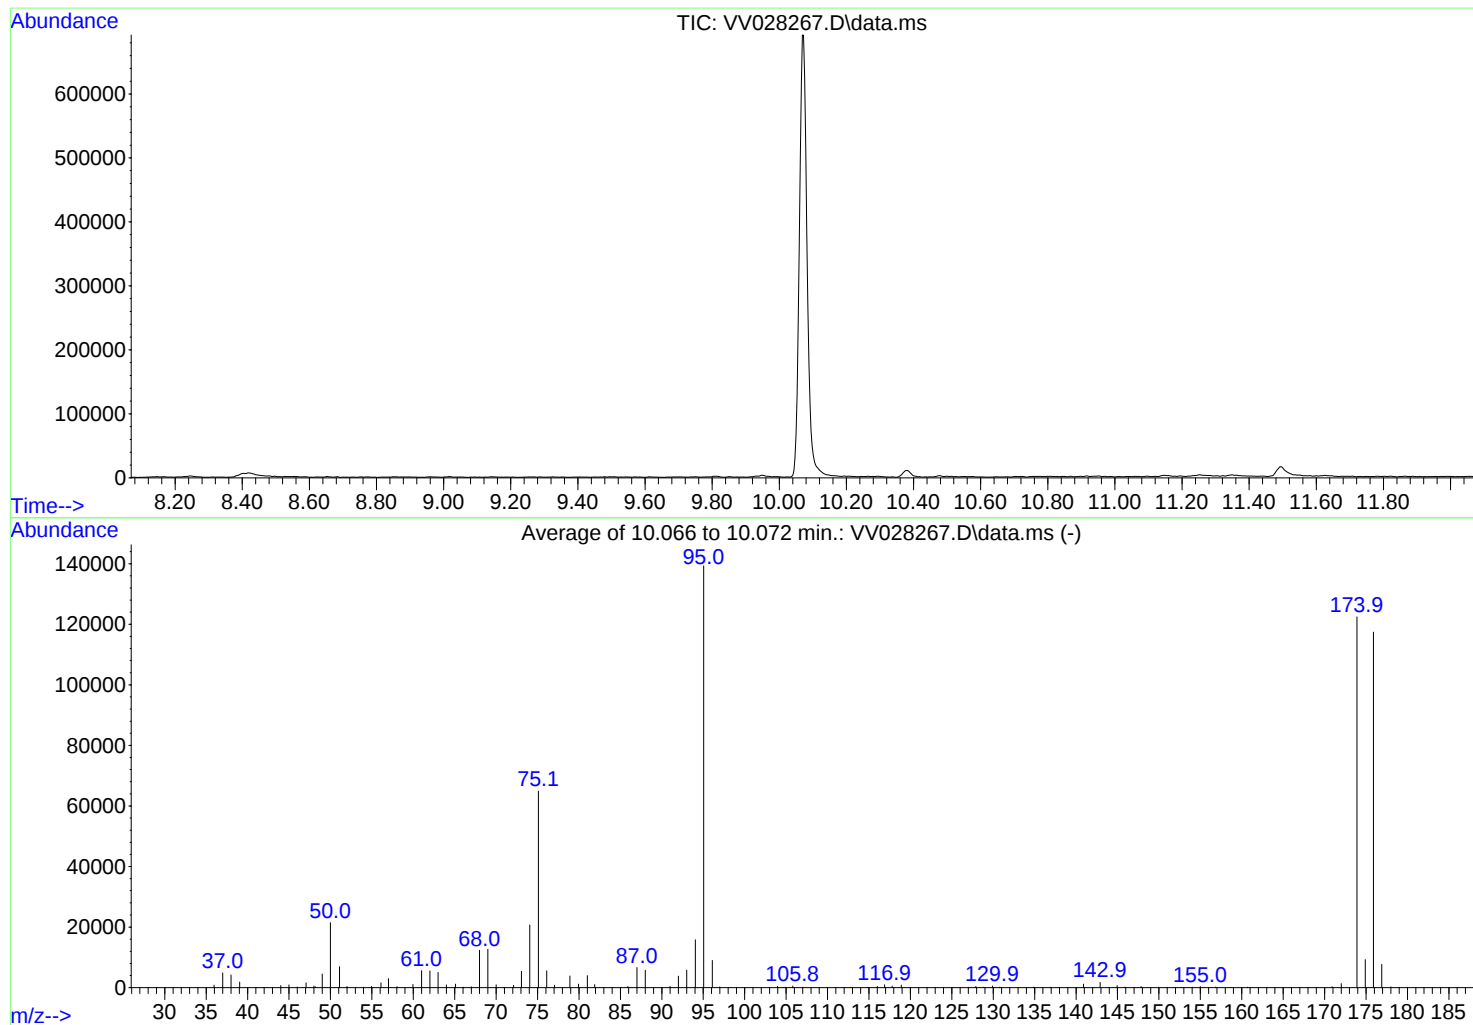

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	21480	PASS
75	95	30	80	46.6	64904	PASS
95	95	100	100	100.0	139299	PASS
96	95	5	9	6.4	8984	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	122440	PASS
175	174	5	9	7.5	9239	PASS
176	174	95	105	95.9	117405	PASS
177	176	5	10	6.6	7734	PASS

m/z	Abundance
40.00	612.0
43.20	114.0
44.00	378.0
54.90	102.0
59.90	118.0
73.00	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
35.90	831.0
37.00	4662.0
38.00	3866.0
39.10	1813.0
39.90	679.0
41.10	126.0
41.90	122.0
44.00	986.0
45.00	894.0
46.10	182.0
47.00	1679.0
48.00	775.0
49.00	4176.0
50.00	20264.0
51.10	6411.0
52.00	376.0
53.00	164.0
54.00	193.0
55.00	490.0
56.10	1481.0
57.00	2649.0
58.00	223.0
60.00	1158.0
61.00	5213.0
62.00	5448.0
63.00	4715.0
64.00	914.0
65.10	1062.0
66.10	180.0
67.00	417.0
68.00	11775.0
69.00	12159.0
70.00	936.0
72.10	659.0
73.10	5523.0
74.10	19024.0
75.10	61504.0
76.10	5237.0
77.00	853.0
78.90	3689.0
79.90	995.0
81.00	3656.0
81.90	950.0
83.00	107.0
85.90	325.0
87.00	6182.0
88.00	5255.0
91.00	385.0
92.00	3563.0
93.00	5465.0
94.00	14490.0
95.00	129704.0
96.10	8374.0
97.00	222.0
104.00	447.0
104.70	168.0
105.00	138.0
105.80	468.0
106.90	168.0
112.80	124.0
114.80	121.0
116.00	469.0
116.90	1032.0
117.80	507.0
118.90	789.0
127.90	398.0
128.80	127.0
129.90	466.0
130.70	230.0
134.90	183.0
136.90	165.0
140.10	126.0
140.90	1069.0
142.90	1555.0
144.90	719.0
145.80	194.0
147.90	332.0
149.10	113.0
149.90	201.0
151.70	111.0
153.00	128.0
154.00	217.0
155.00	335.0
156.80	197.0
160.70	123.0
170.90	324.0
172.00	1172.0
173.90	112216.0
174.90	8825.0
175.90	107504.0
176.90	7104.0
178.00	263.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.00	873.0
37.00	5010.0
38.00	4376.0
39.00	1931.0
39.90	591.0
41.10	110.0
43.10	153.0
44.00	1080.0
45.00	963.0
46.00	217.0
47.10	1660.0
48.00	771.0
49.00	4645.0
50.00	22200.0
51.10	7218.0
52.00	383.0
53.00	162.0
54.00	193.0
55.00	528.0
56.10	1658.0
57.00	3031.0
58.00	325.0
60.00	1225.0
61.00	5796.0
62.00	5711.0
63.00	5232.0
64.00	901.0
65.10	1249.0
66.10	191.0
67.00	447.0
68.00	12680.0
69.00	13139.0
70.00	990.0
72.10	785.0
73.10	5706.0
74.00	21424.0
75.10	67256.0
76.10	5791.0
77.10	846.0
78.90	3975.0
80.00	1169.0
81.00	4167.0
81.90	1089.0
83.00	131.0
85.90	371.0
87.00	7080.0
88.00	5966.0
91.00	421.0
92.00	3933.0
93.00	6047.0
94.10	16200.0
95.10	144704.0
96.10	9251.0
97.00	287.0
104.00	460.0
104.70	171.0
104.90	163.0
105.80	533.0
107.00	192.0
112.80	124.0
114.80	121.0
116.00	437.0
116.90	1009.0
117.80	579.0
118.90	906.0
127.00	102.0
127.90	453.0
128.80	153.0
129.90	600.0
130.80	204.0
134.90	201.0
136.90	186.0
140.90	1189.0
142.90	1789.0
143.90	124.0
145.00	756.0
145.90	227.0
147.80	362.0
149.00	121.0
149.90	199.0
151.70	126.0
153.00	129.0
154.00	211.0
155.00	375.0
156.90	219.0
160.70	151.0
170.90	358.0
172.00	1363.0
173.90	126744.0
174.90	9442.0
175.90	121168.0
176.90	8006.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

178.00

243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.00	934.0
37.00	4847.0
38.00	4367.0
39.00	1885.0
40.00	488.0
43.00	166.0
44.00	1091.0
45.00	923.0
45.90	220.0
47.10	1484.0
48.20	767.0
49.00	4729.0
50.00	21976.0
51.10	7112.0
52.00	332.0
53.10	165.0
54.00	155.0
55.00	461.0
56.10	1704.0
57.00	3149.0
58.10	352.0
60.00	1128.0
61.00	5883.0
62.00	5516.0
63.00	5114.0
64.00	899.0
65.10	1246.0
65.90	187.0
68.00	12440.0
69.00	12751.0
70.00	992.0
70.90	112.0
72.10	810.0
73.10	5523.0
74.00	21752.0
75.10	65952.0
76.10	5656.0
77.10	746.0
78.90	3956.0
80.00	1330.0
81.00	4109.0
81.90	1004.0
83.00	118.0
85.90	368.0
87.00	6787.0
88.00	6015.0
91.00	453.0
92.00	3981.0
93.00	5983.0
94.10	16640.0
95.10	143488.0
96.10	9327.0
97.00	318.0
103.90	391.0
105.00	175.0
105.80	512.0
107.10	165.0
112.80	102.0
114.80	117.0
116.00	427.0
116.90	867.0
117.80	530.0
118.90	940.0
127.90	417.0
128.80	178.0
129.90	565.0
130.90	184.0
134.90	241.0
136.90	186.0
140.90	1236.0
142.10	223.0
142.90	1899.0
143.80	125.0
145.00	639.0
146.00	216.0
146.90	115.0
147.80	365.0
148.90	141.0
150.00	169.0
152.70	134.0
154.00	144.0
155.00	398.0
156.90	230.0
158.60	131.0
160.70	137.0
170.90	368.0
172.00	1384.0
173.90	128360.0
174.90	9451.0
175.90	123544.0
176.90	8091.0
178.00	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381