

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100419\
 Data File : VV013040.D
 Acq On : 04 Oct 2019 11:16
 Operator : SY/MD
 Sample : VV1004SBL01
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK73

Quant Time: Oct 04 18:35:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 04 18:24:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	755068	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	740228	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	360635	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	216097	18.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.76%
7) Chloroethane-d5	1.58	69	197697	20.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.48%
10) 1,1-Dichloroethene-d2	2.13	63	299708	15.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.52%
20) 2-Butanone-d5	3.94	46	171908	42.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.00%
24) Chloroform-d	4.40	84	428892	20.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.72%
26) 1,2-Dichloroethane-d4	5.08	65	254324	21.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.36%
29) Benzene-d6	5.10	84	880104	21.30	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.20%
33) 1,2-Dichloropropane-d6	6.11	67	284774	21.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.92%
37) Toluene-d8	7.36	98	779101	20.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.08%
38) trans-1,3-Dichloropropene-	7.66	79	109446	19.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.80%
39) 2-Hexanone-d5	8.14	63	110157	42.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.52%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	249696	20.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.16%
61) 1,2-Dichlorobenzene-d4	11.67	152	317717	22.68	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.72%


Target Compounds				Ovalue
13) Acetone	2.21	43	9975	2.320 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100419\
Data File : VV013040.D
Acq On : 04 Oct 2019 11:16
Operator : SY/MD
Sample : VV1004SBL01
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK73

Quant Time: Oct 04 18:35:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 04 18:24:09 2019
Response via : Initial Calibration

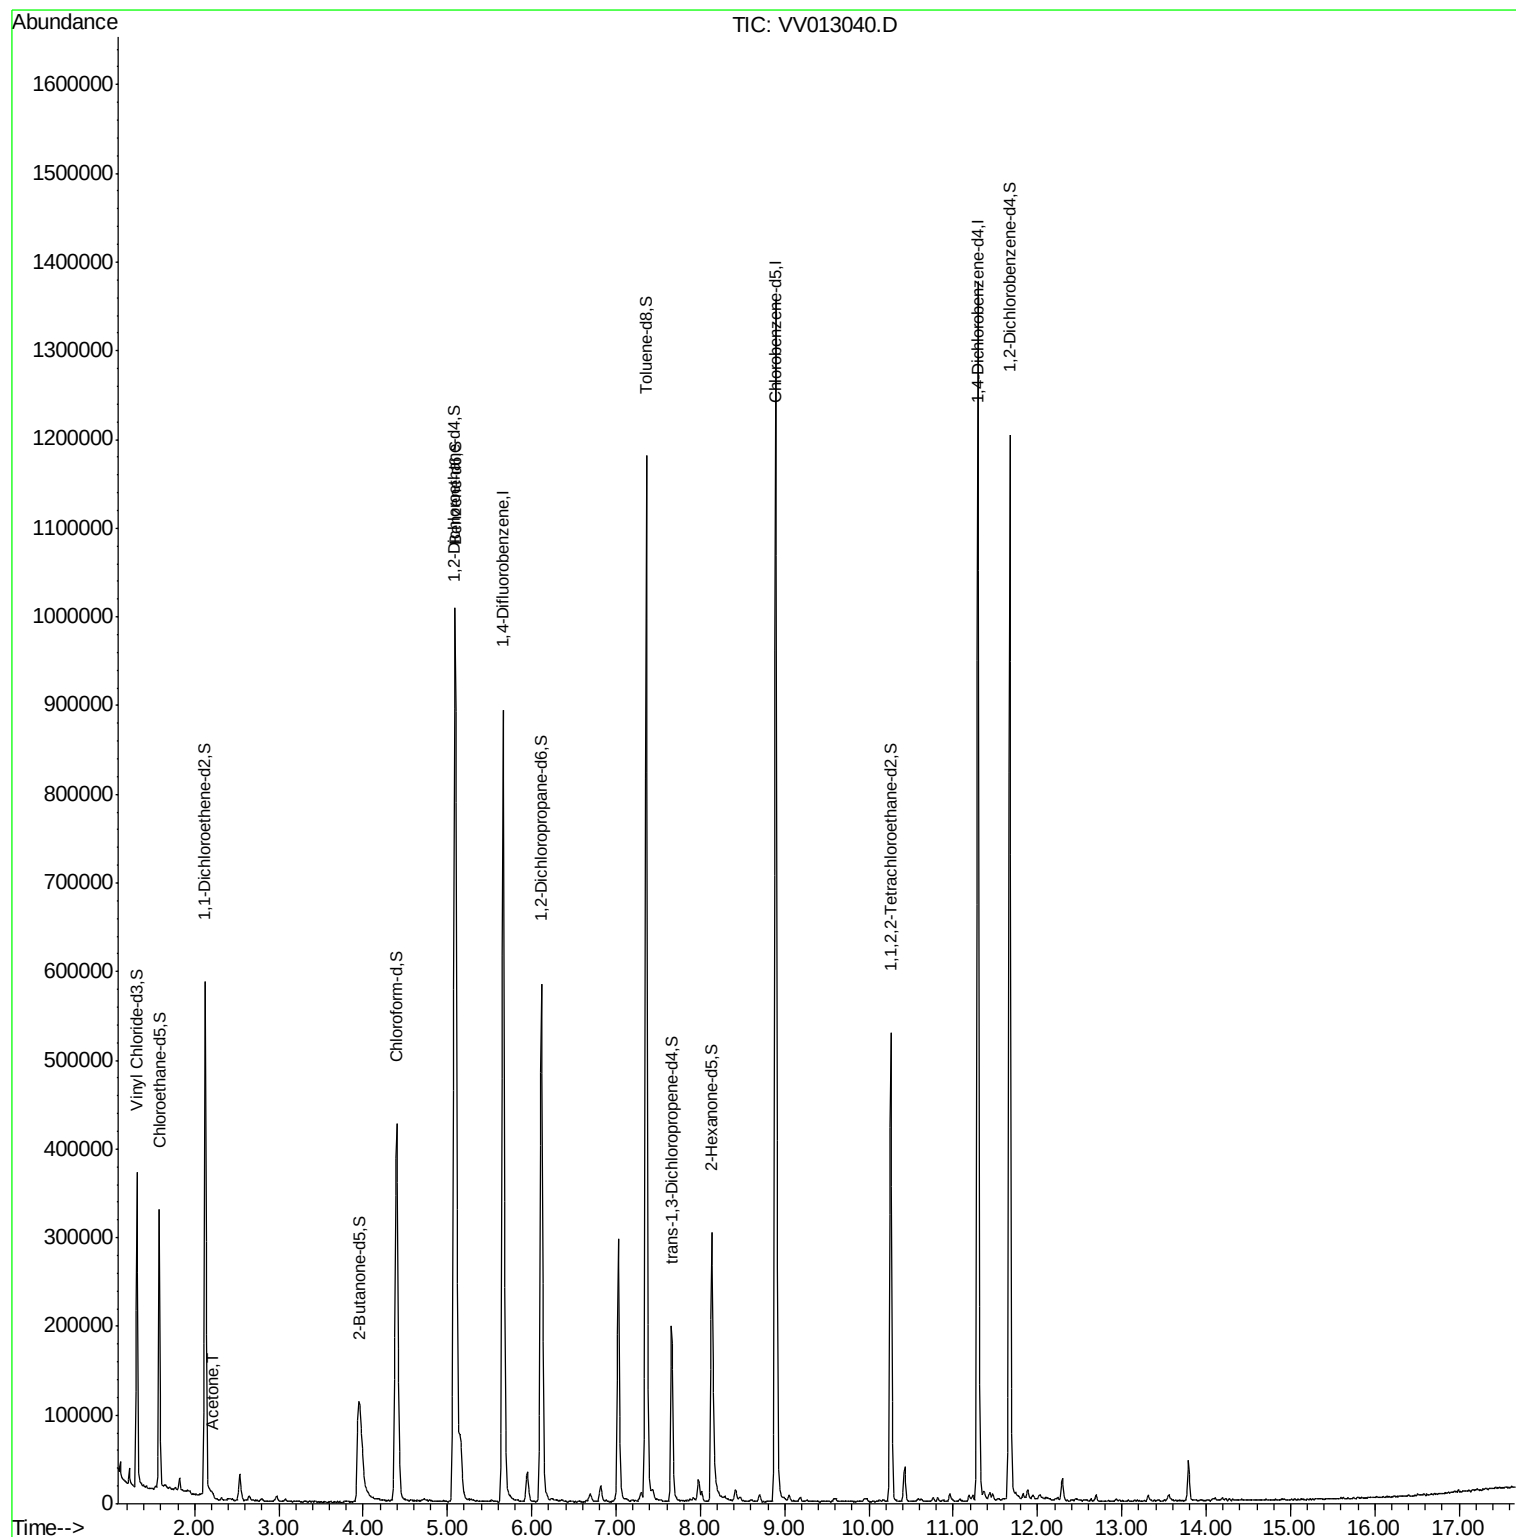

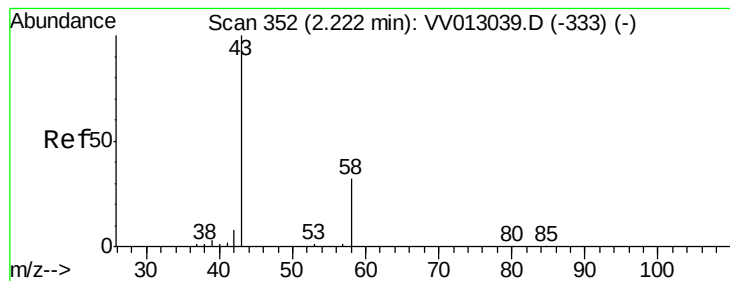

#13

Acetone

Concen: 2.320 ug/L

RT: 2.21 min Scan# 348

Delta R.T. 0.01 min

Lab File: VV013040.D

Acq: 04 Oct 2019 11:16

Instrument :
MSVOA_V
ClientSampleId :
VBLK73

Tot Ion: 43 Resp: 9975

Ion Ratio Lower Upper

43 100

58 35.0 0.0 65.0

