


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100419\
Data File : VV013038.D
Acq On : 04 Oct 2019 09:32
Operator : SY/MD
Sample : BFB66
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Title : VOC Analysis
Last Update : Mon Oct 07 04:06:28 2019

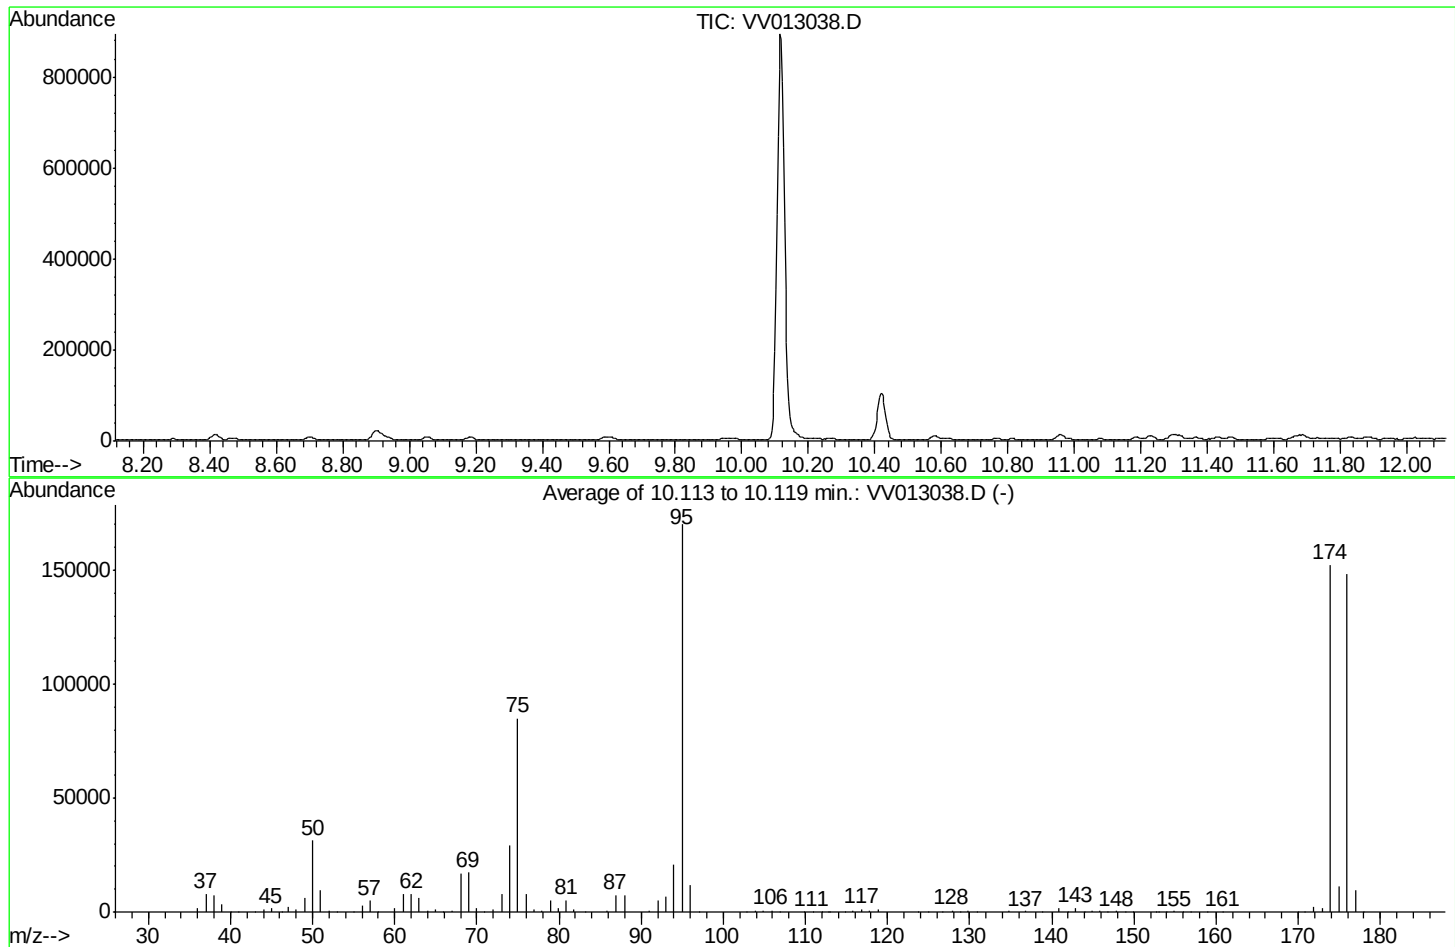

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	31264	PASS
75	95	30	80	50.0	85061	PASS
95	95	100	100	100.0	170154	PASS
96	95	5	9	6.9	11782	PASS
173	174	0.00	2	1.2	1785	PASS
174	95	50	120	89.5	152277	PASS
175	174	5	9	7.5	11492	PASS
176	174	95	101	97.5	148437	PASS
177	176	5	9	6.4	9522	PASS

m/z	Abundance
36.00	1382.0
37.00	7962.0
38.00	6830.0
39.00	3303.0
40.00	1161.0
41.00	106.0
42.90	161.0
44.00	1926.0
45.00	1411.0
46.20	265.0
47.00	2504.0
48.00	837.0
49.00	6204.0
50.00	30360.0
51.00	8703.0
51.90	403.0
53.00	151.0
55.00	480.0
56.00	2752.0
57.00	4458.0
57.90	183.0
60.00	1494.0
61.00	7642.0
62.00	7955.0
63.00	6028.0
64.00	837.0
65.00	1137.0
66.00	166.0
66.90	362.0
68.00	16226.0
69.00	16488.0
70.00	1416.0
72.00	1056.0
73.00	7472.0
74.00	27880.0
75.00	81400.0
76.00	7341.0
76.90	973.0
77.90	670.0
78.90	5100.0
79.90	1632.0
80.90	5021.0
81.90	1169.0
83.10	151.0
85.90	367.0
86.90	7385.0
88.00	6789.0
90.90	693.0
92.00	4741.0
93.00	6442.0
94.00	19696.0
95.00	160896.0
96.00	11441.0
97.00	245.0
102.90	105.0
103.90	698.0
104.80	248.0
105.90	779.0
106.80	228.0
109.80	106.0
110.80	184.0
111.90	148.0
112.80	193.0
114.80	132.0
115.80	633.0
116.90	1159.0
117.80	622.0
118.90	1013.0
123.70	114.0
127.90	588.0
128.80	276.0
129.90	543.0
130.80	260.0
134.80	294.0
136.80	336.0
140.90	1398.0
141.90	207.0
142.90	2030.0
143.90	169.0
144.80	600.0
145.80	340.0
146.80	105.0
147.90	442.0
149.80	223.0
152.70	110.0
153.90	192.0
154.90	359.0
156.00	108.0
156.90	253.0
158.80	239.0
160.80	194.0
170.80	233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

171.90	1983.0
173.00	1598.0
173.90	141056.0
174.90	10878.0
175.90	136128.0
176.90	9046.0
177.90	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	1619.0
37.00	8429.0
38.00	7625.0
39.00	3543.0
39.90	1264.0
41.00	142.0
42.90	182.0
44.00	2024.0
45.00	1494.0
46.20	275.0
47.00	2612.0
47.90	953.0
49.00	6445.0
50.00	32408.0
51.00	9682.0
52.00	407.0
52.90	120.0
55.00	402.0
56.00	3052.0
57.00	5052.0
57.90	170.0
60.00	1504.0
61.00	8259.0
62.00	8332.0
63.00	6289.0
64.00	879.0
65.00	1184.0
65.90	141.0
67.00	420.0
68.00	17560.0
69.00	17992.0
70.00	1537.0
71.90	1048.0
73.00	8086.0
74.00	30384.0
75.00	88008.0
76.00	8106.0
76.90	1050.0
77.90	807.0
78.90	5402.0
79.90	1707.0
80.90	5264.0
81.80	1251.0
83.20	154.0
85.90	393.0
86.90	7776.0
87.90	7501.0
90.90	715.0
92.00	4991.0
93.00	6964.0
94.00	21456.0
95.00	175936.0
96.00	12174.0
97.00	267.0
103.90	764.0
104.90	344.0
105.90	799.0
106.90	227.0
110.90	210.0
112.00	140.0
113.00	152.0
114.70	147.0
115.80	607.0
116.80	1330.0
117.90	617.0
118.90	1027.0
123.70	110.0
127.90	576.0
128.80	280.0
129.90	577.0
130.80	306.0
134.80	325.0
136.80	395.0
138.90	116.0
140.90	1614.0
141.90	198.0
142.90	2045.0
143.90	160.0
144.90	742.0
145.90	341.0
146.80	146.0
147.90	430.0
149.80	222.0
153.00	121.0
153.90	147.0
154.90	426.0
156.90	244.0
158.80	231.0
160.80	212.0
170.80	211.0
171.90	2074.0
173.00	1830.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

173.90	157120.0
174.90	11982.0
175.90	153920.0
176.90	9814.0
177.90	291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	1603.0
37.00	7843.0
38.00	7684.0
39.00	3369.0
39.90	1308.0
41.00	147.0
42.90	192.0
44.00	1948.0
45.00	1481.0
46.20	232.0
47.00	2429.0
47.90	1071.0
49.00	6160.0
50.00	31024.0
51.00	9737.0
52.00	365.0
52.80	119.0
55.00	327.0
56.00	2944.0
57.00	5023.0
57.90	163.0
60.00	1486.0
61.00	8114.0
62.00	7948.0
63.00	6035.0
64.00	814.0
65.00	1253.0
65.90	101.0
67.00	441.0
68.00	17152.0
69.00	17744.0
70.00	1434.0
70.90	106.0
71.90	942.0
73.00	7671.0
74.00	29880.0
75.00	85776.0
76.00	7590.0
77.00	1134.0
77.90	824.0
78.90	5198.0
79.90	1679.0
80.90	5088.0
81.80	1217.0
83.10	143.0
85.90	357.0
86.90	7460.0
87.90	7200.0
90.90	686.0
92.00	4768.0
93.00	6749.0
94.00	21072.0
95.00	173632.0
96.00	11733.0
97.00	303.0
102.80	104.0
103.90	712.0
104.90	378.0
105.90	742.0
106.90	202.0
110.90	184.0
112.00	137.0
113.00	150.0
114.70	166.0
115.80	569.0
116.80	1321.0
117.90	565.0
118.90	874.0
123.80	101.0
124.90	104.0
126.70	105.0
127.90	593.0
128.90	278.0
129.80	613.0
130.80	326.0
134.80	310.0
136.80	341.0
138.80	172.0
140.90	1630.0
141.90	177.0
142.90	1831.0
143.90	121.0
144.90	711.0
145.90	291.0
146.80	162.0
147.90	404.0
148.90	114.0
149.80	202.0
153.00	164.0
153.80	131.0
154.90	498.0
156.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

158.90	227.0
160.80	220.0
169.90	113.0
171.90	1953.0
173.00	1928.0
173.90	158656.0
174.90	11618.0
175.90	155264.0
177.00	9708.0
177.90	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

Scan 2794 (10.074 min): VV013038.D
BFB66

m/z	Abundance
35.70	155.0
39.00	123.0
40.00	1129.0
40.90	102.0
43.10	127.0
44.00	886.0
54.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66