

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037732.D
 Acq On : 04 Oct 2024 09:26
 Operator : SY/MD
 Sample : VV1004WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 07 04:11:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 07 04:10:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	614327	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	601527	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	279164	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	264969	49.134	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 98.260%			
7) Chloroethane-d5	1.535	69	218221	52.132	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 104.260%			
11) 1,1-Dichloroethene-d2	2.063	65	115053	51.065	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 102.140%			
21) 2-Butanone-d5	3.796	46	197530	102.836	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 102.840%			
24) Chloroform-d	4.246	84	491205	51.197	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.400%			
26) 1,2-Dichloroethane-d4	4.937	65	302646	53.891	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.780%			
32) Benzene-d6	4.953	84	986807	52.426	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.860%			
36) 1,2-Dichloropropane-d6	5.985	67	316450	52.796	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 105.600%			
41) Toluene-d8	7.236	98	860810	50.434	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 100.860%			
43) trans-1,3-Dichloroprop...	7.548	79	134822	48.421	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 96.840%			
47) 2-Hexanone-d5	8.024	63	116351	91.930	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 91.930%			
56) 1,1,2,2-Tetrachloroeth...	10.146	84	348492	50.039	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 100.080%			
66) 1,2-Dichlorobenzene-d4	11.554	152	325857	55.394	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.780%			
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3521	0.804	ug/L	# 26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037732.D
Acq On : 04 Oct 2024 09:26
Operator : SY/MD
Sample : VV1004WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 07 04:11:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 07 04:10:13 2024
Response via : Initial Calibration

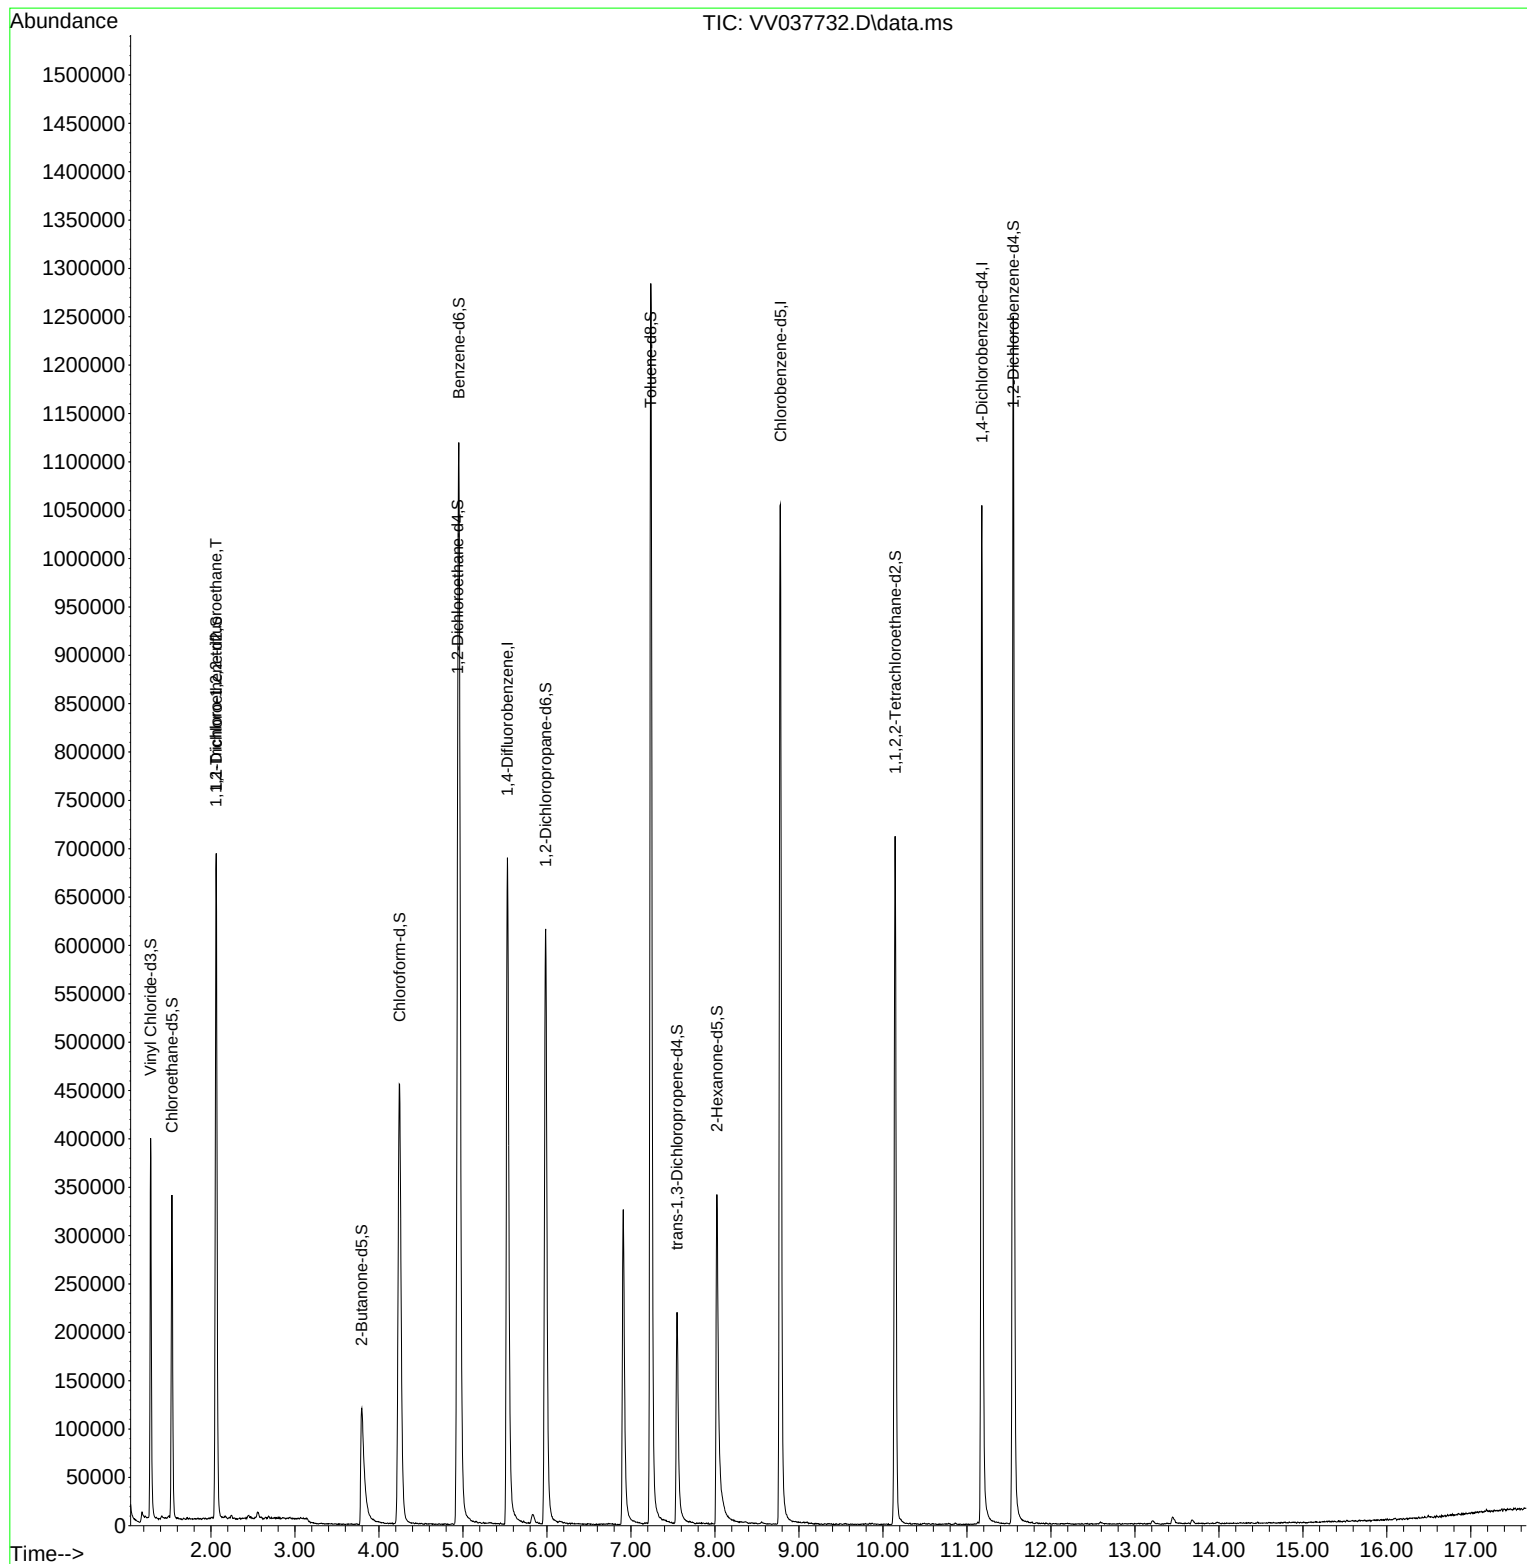

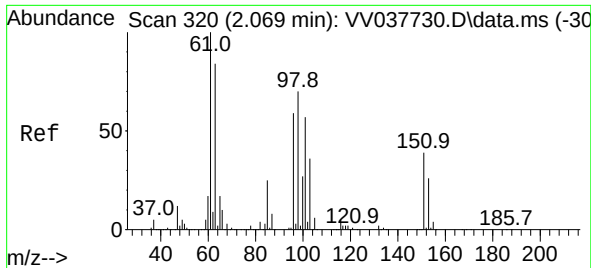

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.804 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV037732.D
 Acq: 04 Oct 2024 09:26

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion:101 Resp: 3521
 Ion Ratio Lower Upper
 101 100
 85 3.1 34.6 52.0#
 151 4.7 57.5 86.3#

