

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037735.D
 Acq On : 04 Oct 2024 10:54
 Operator : SY/MD
 Sample : P4238-01ME
 Misc : 4.61G/5mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 07 04:11:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 07 04:10:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.523	114	618654	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	601229	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	285134	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	188569	34.722	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.440%
7) Chloroethane-d5	1.503	69	67839	16.093	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	32.180%#
11) 1,1-Dichloroethene-d2	2.044	65	86689	38.207	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.420%
21) 2-Butanone-d5	3.799	46	151923	78.540	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.540%
24) Chloroform-d	4.233	84	379100	39.236	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.480%
26) 1,2-Dichloroethane-d4	4.931	65	236943	41.896	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.800%
32) Benzene-d6	4.944	84	757201	40.247	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.500%
36) 1,2-Dichloropropane-d6	5.979	67	249533	41.653	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.300%
41) Toluene-d8	7.233	98	663464	38.891	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.780%#
43) trans-1,3-Dichloroprop...	7.548	79	106109	38.128	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.260%
47) 2-Hexanone-d5	8.024	63	95616	75.585	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.580%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	272707	39.177	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.360%
66) 1,2-Dichlorobenzene-d4	11.555	152	268690	44.719	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.440%
Target Compounds						
39) cis-1,3-Dichloropropene	6.905	75	6373	0.853	ug/L	Qvalue # 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037735.D
Acq On : 04 Oct 2024 10:54
Operator : SY/MD
Sample : P4238-01ME
Misc : 4.61G/5mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 07 04:11:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 07 04:10:13 2024
Response via : Initial Calibration

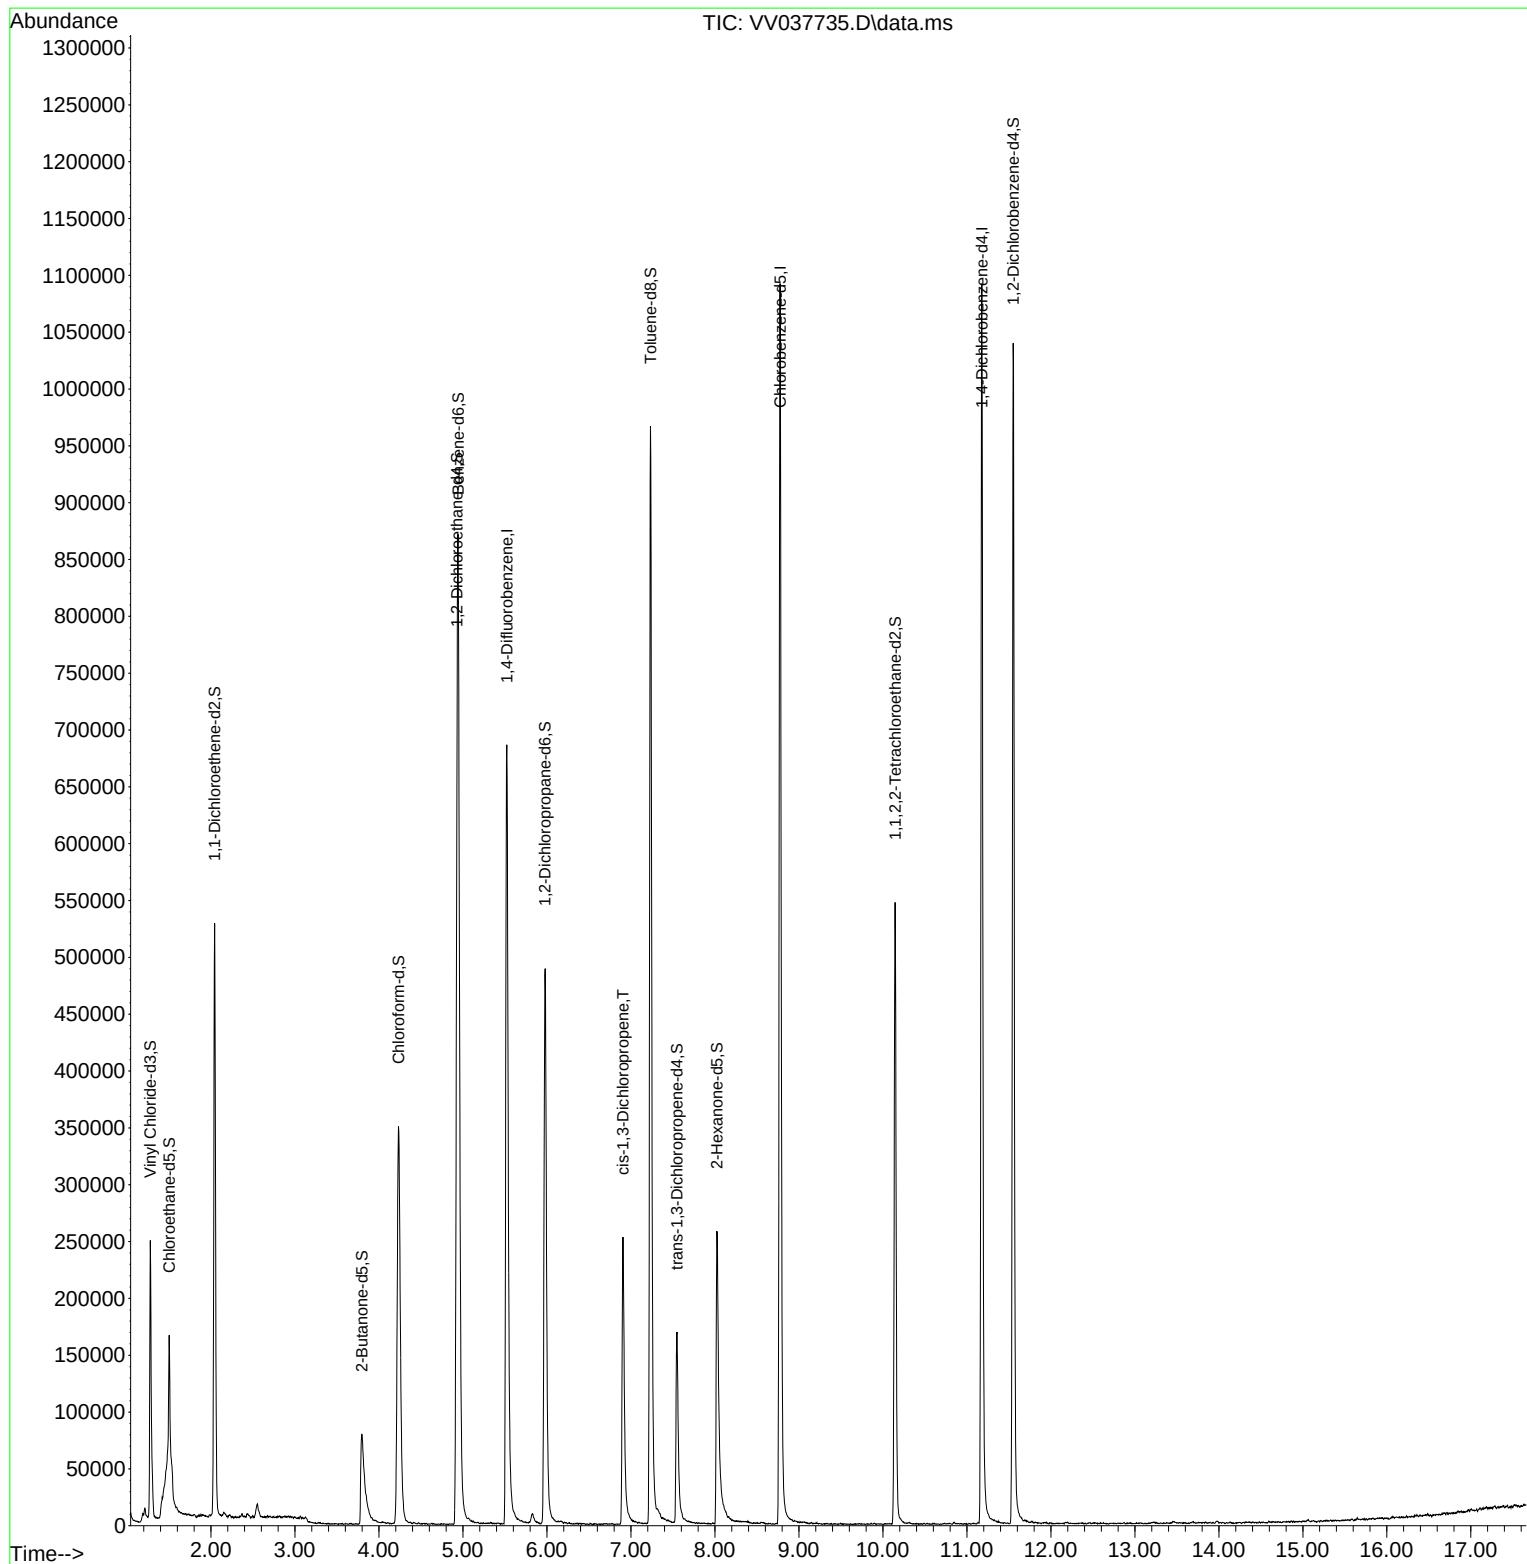

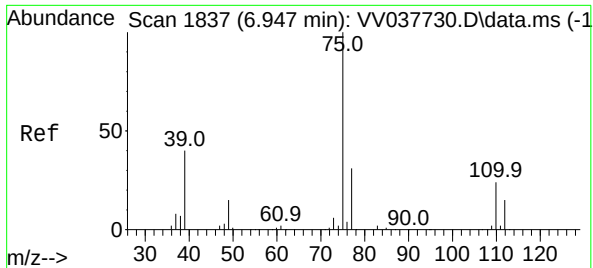

#39
 cis-1,3-Dichloropropene
 Concen: 0.853 ug/L
 RT: 6.905 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV037735.D
 Acq: 04 Oct 2024 10:54

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6373
 Ion Ratio Lower Upper
 75 100
 77 52.4 21.8 40.4#

