

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037737.D
 Acq On : 04 Oct 2024 11:37
 Operator : SY/MD
 Sample : P4238-03ME
 Misc : 5.30G/5mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 07 04:12:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 07 04:10:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	610231	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	598429	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	280849	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	185536	34.635	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.280%
7) Chloroethane-d5	1.503	69	69357	16.680	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	33.360%#
11) 1,1-Dichloroethene-d2	2.047	65	85512	38.208	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.420%
21) 2-Butanone-d5	3.799	46	170613	89.419	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.420%
24) Chloroform-d	4.239	84	389711	40.891	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.780%
26) 1,2-Dichloroethane-d4	4.934	65	245971	44.093	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.180%
32) Benzene-d6	4.947	84	772137	41.233	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.460%
36) 1,2-Dichloropropane-d6	5.982	67	253080	42.442	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.880%
41) Toluene-d8	7.236	98	670060	39.461	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.920%#
43) trans-1,3-Dichloroprop...	7.548	79	105009	37.909	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.820%
47) 2-Hexanone-d5	8.027	63	106341	84.456	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.460%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	286649	41.373	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.740%
66) 1,2-Dichlorobenzene-d4	11.554	152	273578	46.228	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.460%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.371	43	7919	2.426	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037737.D
Acq On : 04 Oct 2024 11:37
Operator : SY/MD
Sample : P4238-03ME
Misc : 5.30G/5mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 07 04:12:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 07 04:10:13 2024
Response via : Initial Calibration

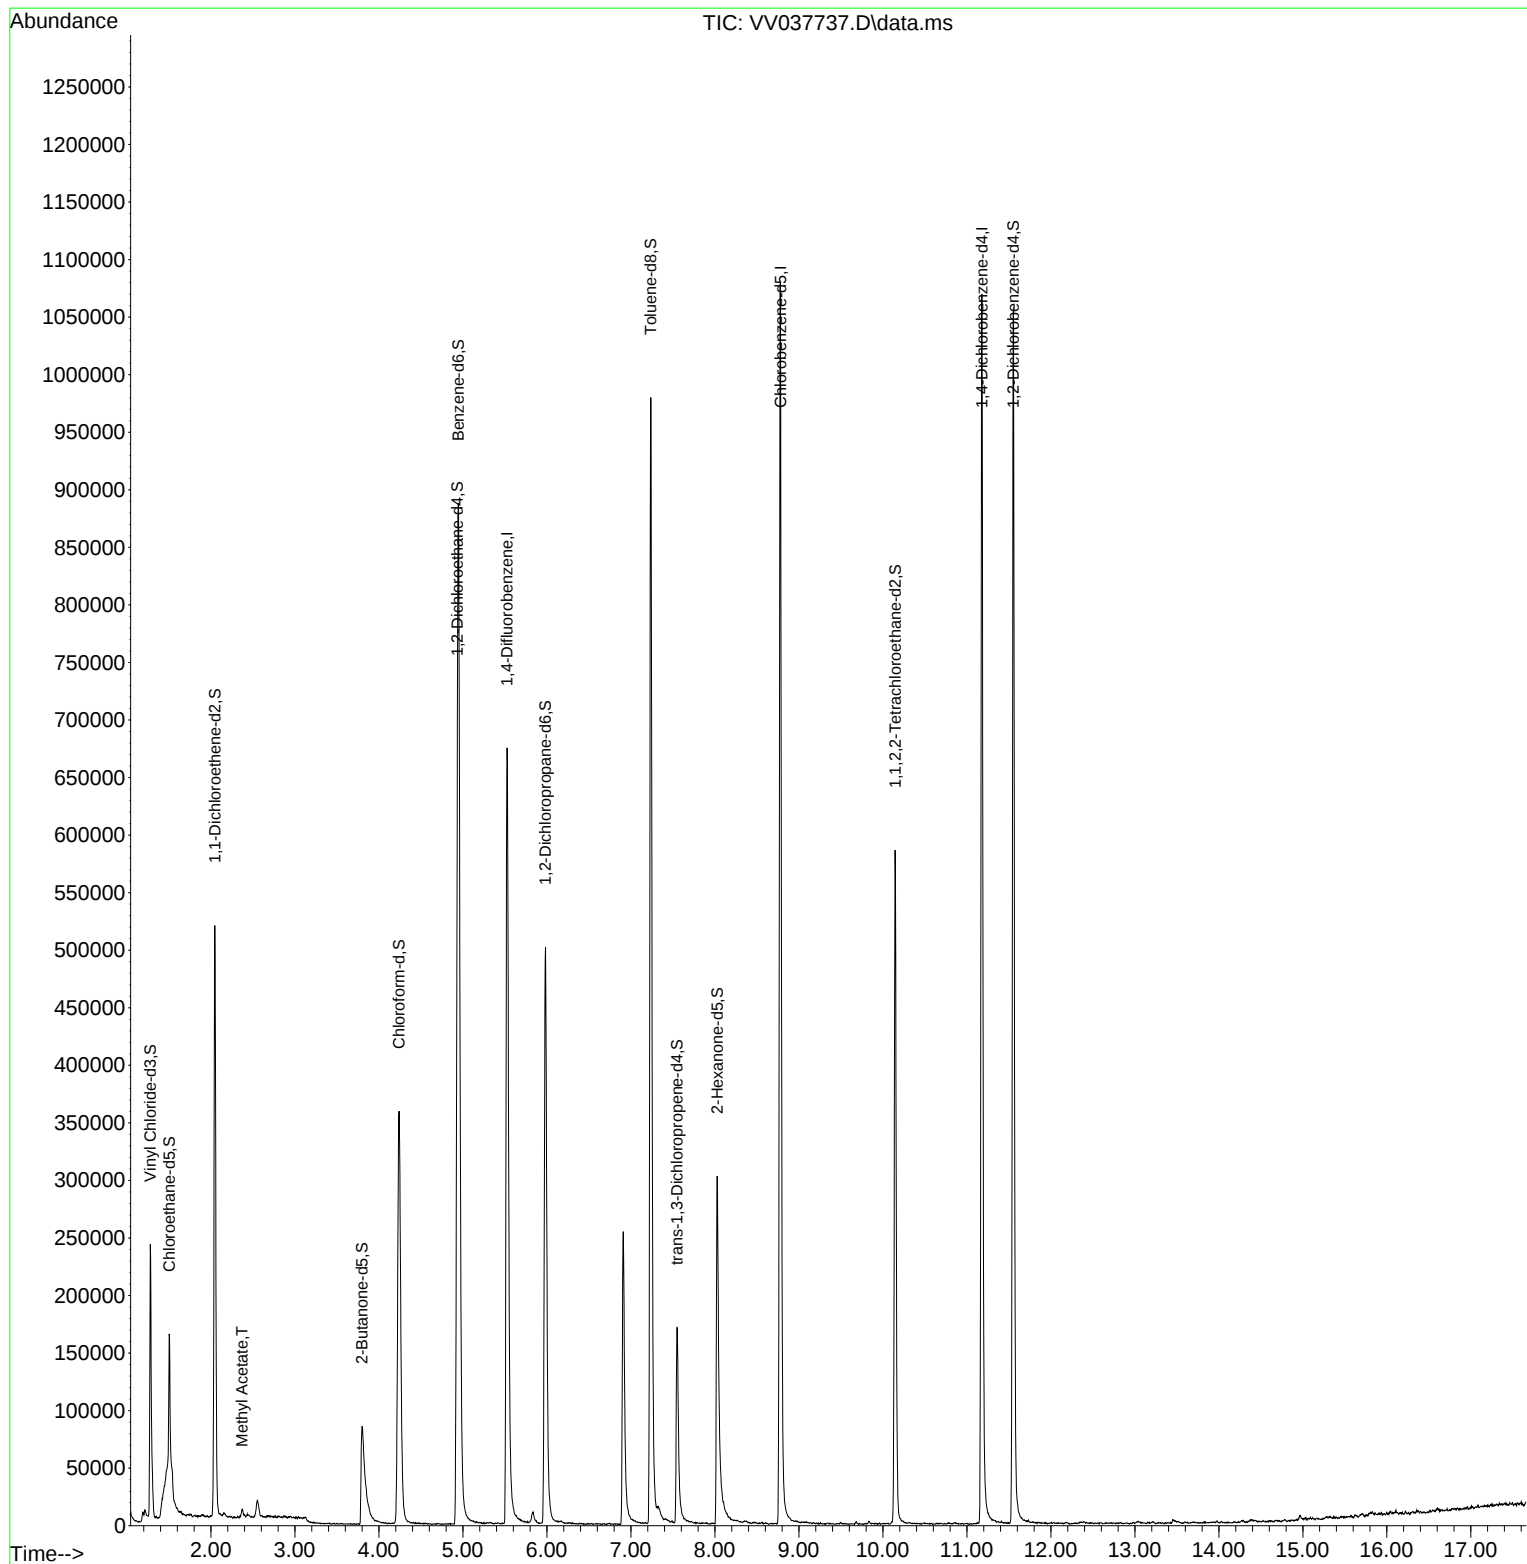

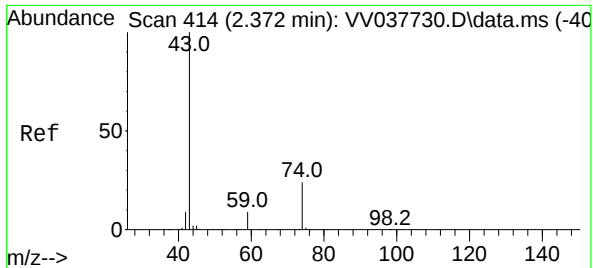

#15
Methyl Acetate
Concen: 2.426 ug/L
RT: 2.371 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV037737.D
Acq: 04 Oct 2024 11:37

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 43 Resp: 7919
Ion Ratio Lower Upper
43 100
74 28.0 19.4 29.0

