

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037743.D
 Acq On : 04 Oct 2024 15:27
 Operator : SY/MD
 Sample : P4284-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 07 04:13:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 07 04:10:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	598875	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	589298	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	275127	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	248965	47.357	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.720%		
7) Chloroethane-d5	1.532	69	205220	50.291	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	100.580%		
11) 1,1-Dichloroethene-d2	2.060	65	107018	48.724	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.440%		
21) 2-Butanone-d5	3.796	46	185222	98.917	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.920%		
24) Chloroform-d	4.243	84	460922	49.280	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.560%		
26) 1,2-Dichloroethane-d4	4.937	65	283566	51.796	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.600%		
32) Benzene-d6	4.953	84	908210	49.251	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.500%		
36) 1,2-Dichloropropane-d6	5.982	67	290786	49.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.040%		
41) Toluene-d8	7.236	98	783631	46.865	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.720%		
43) trans-1,3-Dichloroprop...	7.551	79	124219	45.539	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.080%		
47) 2-Hexanone-d5	8.024	63	108102	87.185	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.190%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	327564	48.010	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.020%		
66) 1,2-Dichlorobenzene-d4	11.554	152	303683	52.382	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.760%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3154	0.739	ug/L	# 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037743.D
Acq On : 04 Oct 2024 15:27
Operator : SY/MD
Sample : P4284-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 07 04:13:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 07 04:10:13 2024
Response via : Initial Calibration

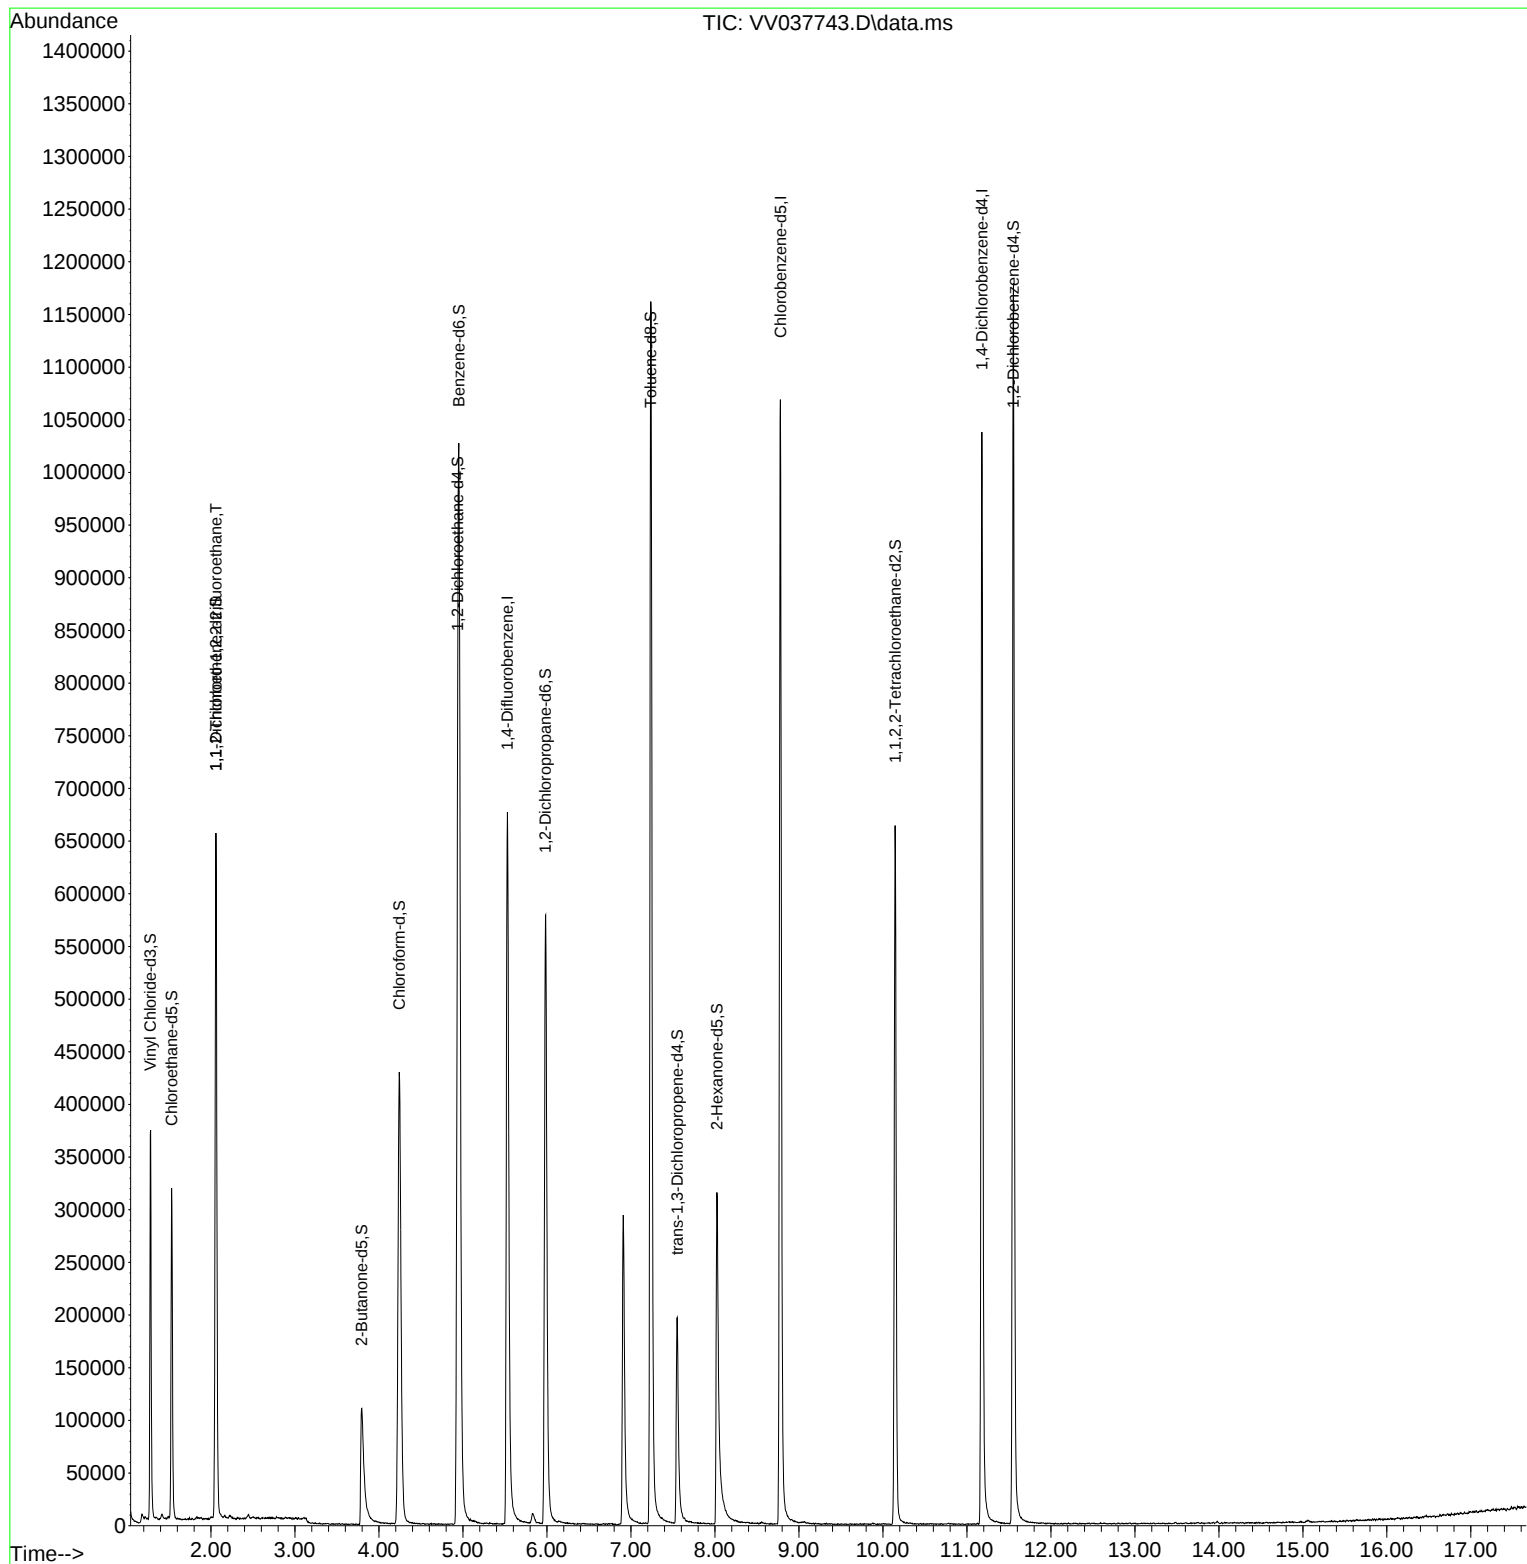

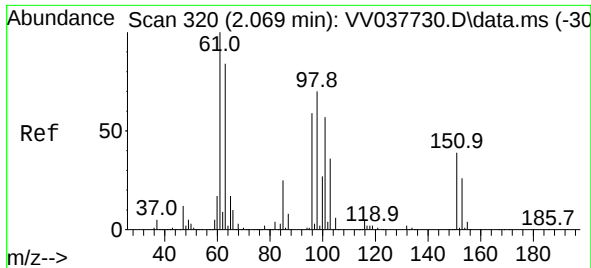

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.739 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV037743.D
 Acq: 04 Oct 2024 15:27

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion:101 Resp: 3154
 Ion Ratio Lower Upper
 101 100
 85 5.2 34.6 52.0#
 151 0.7 57.5 86.3#

