

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037740.D
 Acq On : 04 Oct 2024 13:56
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Quant Time: Oct 07 04:12:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 07 04:10:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	633116	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	620681	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	287542	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	196059	35.277	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.560%		
7) Chloroethane-d5	1.532	69	171794	39.823	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.640%		
11) 1,1-Dichloroethene-d2	2.060	65	88546	38.134	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.260%		
21) 2-Butanone-d5	3.793	46	171018	86.392	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.390%		
24) Chloroform-d	4.243	84	412905	41.759	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.520%		
26) 1,2-Dichloroethane-d4	4.937	65	247400	42.746	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.500%		
32) Benzene-d6	4.953	84	785343	40.435	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.880%		
36) 1,2-Dichloropropane-d6	5.982	67	257764	41.678	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.360%		
41) Toluene-d8	7.236	98	678417	38.521	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.040%#		
43) trans-1,3-Dichloroprop...	7.551	79	107156	37.297	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.600%		
47) 2-Hexanone-d5	8.024	63	100706	77.114	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.110%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	289950	40.349	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.700%		
66) 1,2-Dichlorobenzene-d4	11.551	152	268976	44.392	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.780%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	62424	32.168	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037740.D
Acq On : 04 Oct 2024 13:56
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Time: Oct 07 04:12:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 07 04:10:13 2024
Response via : Initial Calibration

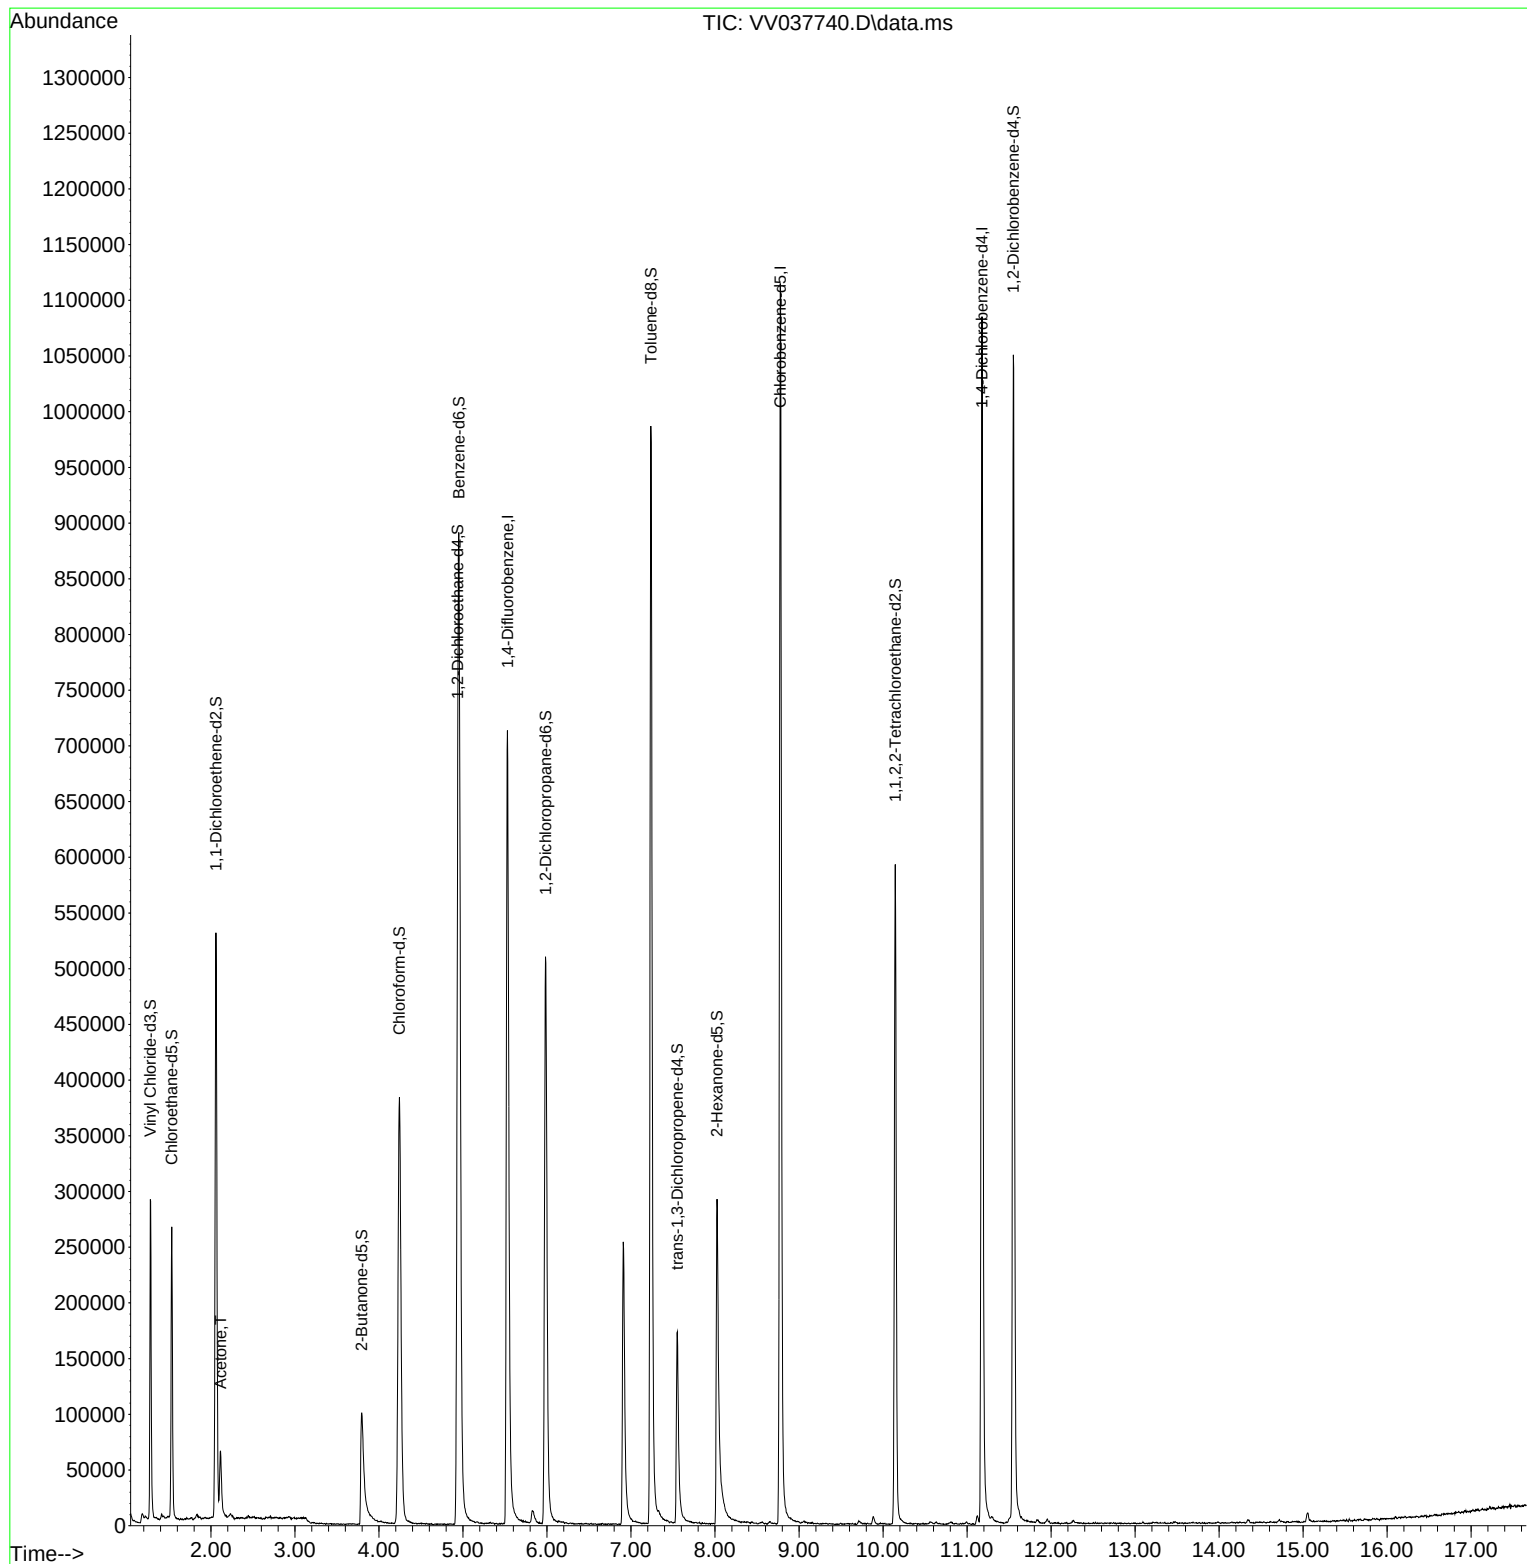

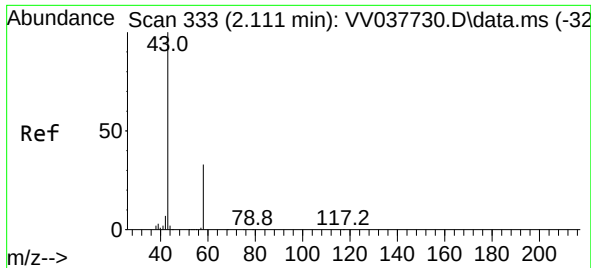

#13
Acetone
Concen: 32.168 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV037740.D
Acq: 04 Oct 2024 13:56

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Tgt Ion: 43 Resp: 62424
Ion Ratio Lower Upper
43 100
58 32.5 0.0 66.6

