

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037732.D
 Acq On : 04 Oct 2024 09:26
 Operator : SY/MD
 Sample : VV1004WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	94	rVB	392742	424239	14.96%	2.162%
2	1.535	147	154	172	rVB	334545	397975	14.04%	2.028%
3	2.063	308	318	338	rBV	686863	996502	35.15%	5.079%
4	3.497	762	764	767	rVB2	410	200	0.01%	0.001%
5	3.513	767	769	770	rBV	421	183	0.01%	0.001%
6	3.571	784	787	794	rBV4	712	559	0.02%	0.003%
7	3.619	798	802	804	rBV2	586	415	0.01%	0.002%
8	3.632	804	806	808	rVB2	574	178	0.01%	0.001%
9	3.709	827	830	832	rBV3	482	249	0.01%	0.001%
10	3.735	834	838	840	rVB2	523	401	0.01%	0.002%
11	3.796	848	857	893	rBV	120020	370279	13.06%	1.887%
12	4.243	981	996	1032	rBV	453932	1156381	40.79%	5.893%
13	4.548	1088	1091	1096	rBV4	1015	972	0.03%	0.005%
14	4.638	1118	1119	1121	rBV	466	142	0.01%	0.001%
15	4.674	1128	1130	1133	rBV2	409	262	0.01%	0.001%
16	4.709	1139	1141	1143	rBV2	572	363	0.01%	0.002%
17	4.764	1156	1158	1160	rBV3	818	313	0.01%	0.002%
18	4.783	1160	1164	1165	rBV3	859	535	0.02%	0.003%
19	4.809	1170	1172	1175	rBV2	252	159	0.01%	0.001%
20	4.950	1200	1216	1252	rBV2	1118124	2835123	100.00%	14.449%
21	5.449	1367	1371	1376	rBV4	1339	1100	0.04%	0.006%
22	5.529	1385	1396	1434	rBV	688797	1435814	50.64%	7.317%
23	5.985	1525	1538	1567	rBV	614983	1289756	45.49%	6.573%
24	6.468	1687	1688	1690	rVB2	398	146	0.01%	0.001%
25	6.487	1690	1694	1698	rBV4	924	1065	0.04%	0.005%
26	6.522	1703	1705	1706	rBV2	632	213	0.01%	0.001%
27	6.587	1723	1725	1728	rVV2	772	369	0.01%	0.002%
28	6.603	1728	1730	1732	rBV	307	160	0.01%	0.001%
29	6.641	1737	1742	1743	rBV2	585	455	0.02%	0.002%
30	6.674	1749	1752	1754	rBV3	458	230	0.01%	0.001%
31	6.731	1768	1770	1773	rBV3	771	478	0.02%	0.002%
32	6.805	1791	1793	1795	rBV2	579	278	0.01%	0.001%
33	6.860	1807	1810	1811	rBV2	367	156	0.01%	0.001%
34	6.908	1815	1825	1862	rBV	325453	623642	22.00%	3.178%
35	7.236	1916	1927	1962	rBV	1282231	2257871	79.64%	11.507%
36	7.548	2015	2024	2055	rBV	217737	406948	14.35%	2.074%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037732.D
 Acq On : 04 Oct 2024 09:26
 Operator : SY/MD
 Sample : VV1004WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.944	2145	2147	2148	rBV2	559	216	0.01%	0.001%
38	7.963	2151	2153	2155	rBV3	1034	421	0.01%	0.002%
39	8.024	2163	2172	2211	rBV2	340943	745678	26.30%	3.800%
40	8.780	2396	2407	2440	rBV	1053933	1796557	63.37%	9.156%
41	9.185	2531	2533	2535	rVB3	721	290	0.01%	0.001%
42	9.201	2535	2538	2542	rBV5	1023	798	0.03%	0.004%
43	9.291	2562	2566	2567	rBV2	379	290	0.01%	0.001%
44	9.304	2567	2570	2574	rBV4	800	625	0.02%	0.003%
45	9.345	2579	2583	2586	rBV5	1240	1119	0.04%	0.006%
46	9.362	2586	2588	2593	rVB3	565	430	0.02%	0.002%
47	9.410	2599	2603	2606	rVB4	694	444	0.02%	0.002%
48	9.426	2606	2608	2610	rBV2	332	189	0.01%	0.001%
49	9.439	2610	2612	2614	rBV2	563	347	0.01%	0.002%
50	9.480	2623	2625	2626	rBV2	715	284	0.01%	0.001%
51	9.612	2664	2666	2668	rBV2	485	210	0.01%	0.001%
52	9.696	2689	2692	2696	rBV2	499	504	0.02%	0.003%
53	9.751	2706	2709	2711	rBV2	453	359	0.01%	0.002%
54	9.789	2719	2721	2725	rVB3	718	362	0.01%	0.002%
55	9.844	2735	2738	2742	rVB2	1135	752	0.03%	0.004%
56	9.870	2743	2746	2754	rVB5	1222	1256	0.04%	0.006%
57	9.902	2754	2756	2763	rVB4	637	704	0.02%	0.004%
58	9.931	2763	2765	2768	rBV3	597	441	0.02%	0.002%
59	9.982	2777	2781	2783	rVB4	501	351	0.01%	0.002%
60	10.001	2783	2787	2788	rBV2	587	363	0.01%	0.002%
61	10.011	2788	2790	2795	rVV4	343	304	0.01%	0.002%
62	10.066	2804	2807	2809	rVB	1058	517	0.02%	0.003%
63	10.085	2809	2813	2814	rBV2	309	223	0.01%	0.001%
64	10.146	2819	2832	2858	rBV	711271	1128119	39.79%	5.749%
65	10.355	2894	2897	2898	rBV	562	304	0.01%	0.002%
66	10.407	2911	2913	2916	rBV3	533	293	0.01%	0.001%
67	10.445	2923	2925	2926	rVB	550	154	0.01%	0.001%
68	10.471	2930	2933	2935	rBV2	778	525	0.02%	0.003%
69	10.587	2966	2969	2970	rBV2	616	385	0.01%	0.002%
70	10.667	2991	2994	2996	rBV2	747	379	0.01%	0.002%
71	10.689	2999	3001	3005	rVV3	416	228	0.01%	0.001%
72	10.709	3005	3007	3010	rBV3	389	203	0.01%	0.001%
73	10.760	3020	3023	3025	rBV2	589	293	0.01%	0.001%
74	10.783	3028	3030	3035	rVV3	917	585	0.02%	0.003%
75	10.841	3045	3048	3049	rBV	481	288	0.01%	0.001%
76	10.860	3051	3054	3056	rBV2	1153	732	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037732.D
 Acq On : 04 Oct 2024 09:26
 Operator : SY/MD
 Sample : VV1004WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.915	3068	3071	3072	rBV2	434	240	0.01%	0.001%
78	10.956	3080	3084	3086	rBV3	355	297	0.01%	0.002%
79	10.988	3092	3094	3099	rBV2	636	291	0.01%	0.001%
80	11.033	3106	3108	3109	rBV2	343	144	0.01%	0.001%
81	11.178	3142	3153	3183	rBV	1052246	1675739	59.11%	8.540%
82	11.551	3256	3269	3300	rBV	1248939	2015961	71.11%	10.274%
83	11.940	3386	3390	3392	rBV3	1045	865	0.03%	0.004%
84	11.988	3401	3405	3407	rBV4	1107	765	0.03%	0.004%
85	12.030	3413	3418	3423	rBV5	878	1259	0.04%	0.006%
86	12.278	3493	3495	3498	rVB2	483	267	0.01%	0.001%
87	12.297	3498	3501	3504	rBV3	744	509	0.02%	0.003%
88	12.326	3504	3510	3514	rVV4	710	872	0.03%	0.004%
89	12.345	3514	3516	3520	rVV2	733	347	0.01%	0.002%
90	12.368	3521	3523	3527	rVB3	880	547	0.02%	0.003%
91	12.435	3542	3544	3550	rVB4	1071	783	0.03%	0.004%
92	12.590	3586	3592	3596	rBV6	1933	2344	0.08%	0.012%
93	12.699	3624	3626	3629	rBV4	506	300	0.01%	0.002%
94	12.792	3653	3655	3657	rBV	449	237	0.01%	0.001%
95	13.140	3761	3763	3766	rBV2	694	499	0.02%	0.003%
96	13.213	3778	3786	3795	rBV9	3192	6642	0.23%	0.034%
97	13.355	3826	3830	3835	rBV3	798	945	0.03%	0.005%
98	13.448	3852	3859	3866	rBV2	6944	13052	0.46%	0.067%
99	13.596	3903	3905	3908	rBV3	848	469	0.02%	0.002%
100	13.680	3925	3931	3945	rBV9	3897	7760	0.27%	0.040%




Sum of corrected areas: 19621767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037732.D
Acq On : 04 Oct 2024 09:26
Operator : SY/MD
Sample : VV1004WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

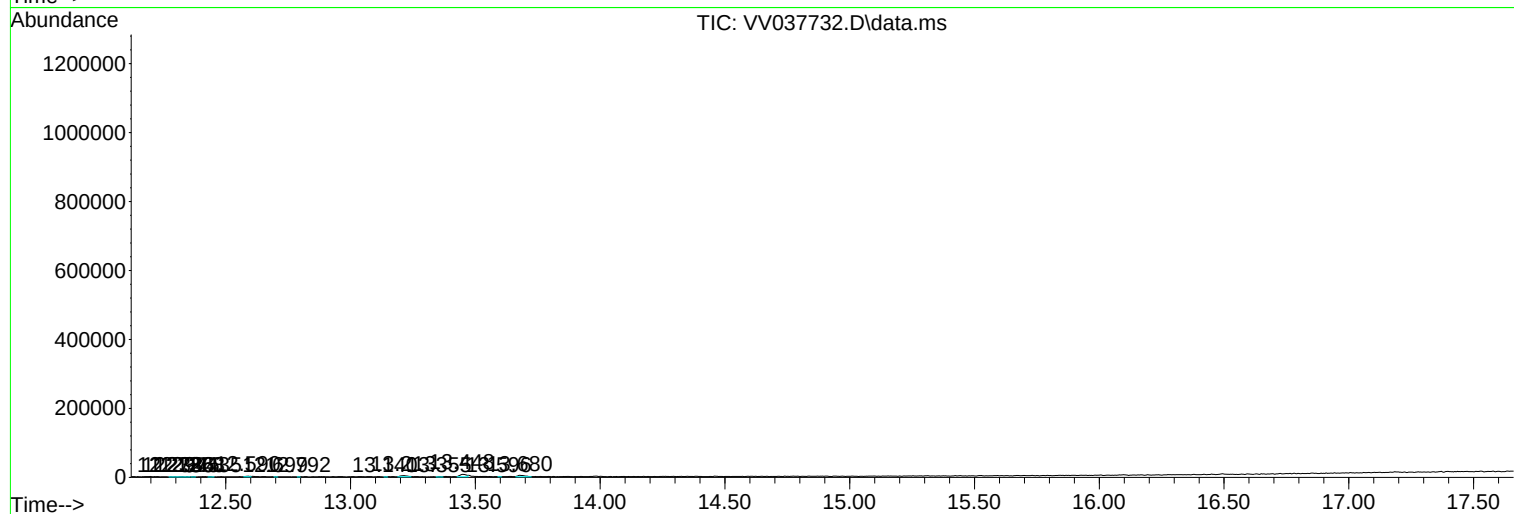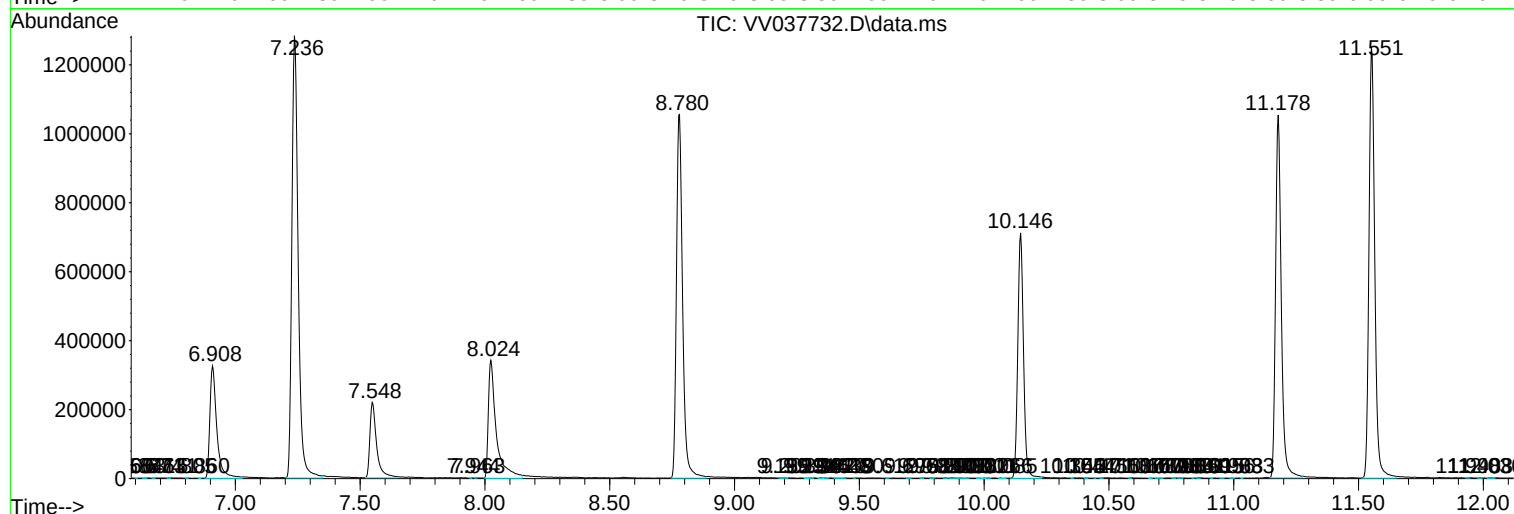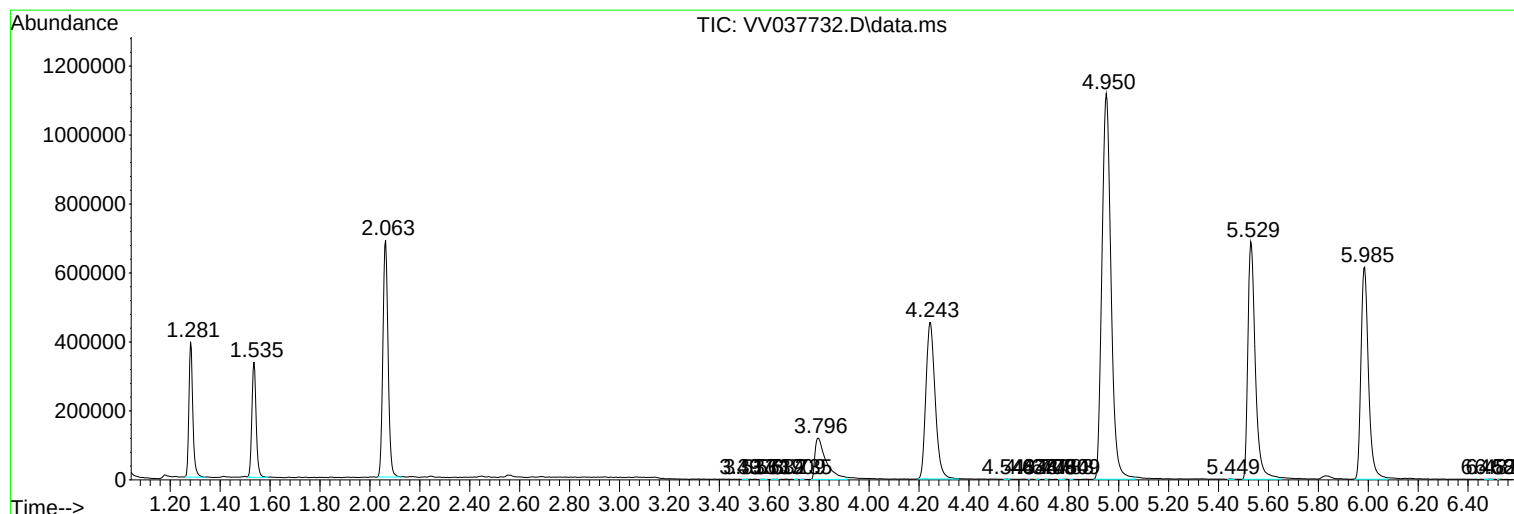

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037732.D
Acq On : 04 Oct 2024 09:26
Operator : SY/MD
Sample : VV1004WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037732.D
Acq On : 04 Oct 2024 09:26
Operator : SY/MD
Sample : VV1004WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------