

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037733.D
 Acq On : 04 Oct 2024 09:47
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	35	43	51	rBV	11240	20372	0.77%	0.109%
2	1.278	67	74	87	rBV	367956	397575	15.07%	2.123%
3	1.532	145	153	166	rVB	312046	365960	13.87%	1.954%
4	2.060	307	317	332	rBV	646060	929966	35.24%	4.966%
5	3.410	734	737	741	rBV5	691	488	0.02%	0.003%
6	3.468	748	755	758	rBV2	711	693	0.03%	0.004%
7	3.503	762	766	768	rBV	858	463	0.02%	0.002%
8	3.683	817	822	827	rVB5	851	966	0.04%	0.005%
9	3.719	830	833	837	rVB2	707	622	0.02%	0.003%
10	3.793	847	856	900	rBV	111597	329591	12.49%	1.760%
11	4.124	954	959	960	rBV3	764	574	0.02%	0.003%
12	4.243	979	996	1029	rBV	420154	1083617	41.06%	5.787%
13	4.593	1103	1105	1108	rVB2	943	471	0.02%	0.003%
14	4.654	1122	1124	1128	rBV4	919	795	0.03%	0.004%
15	4.738	1147	1150	1157	rVB7	780	743	0.03%	0.004%
16	4.767	1157	1159	1163	rBV3	670	481	0.02%	0.003%
17	4.806	1169	1171	1174	rBV	660	487	0.02%	0.003%
18	4.950	1200	1216	1254	rBV2	1030710	2639009	100.00%	14.093%
19	5.207	1294	1296	1299	rBV2	830	521	0.02%	0.003%
20	5.310	1325	1328	1330	rBV4	995	671	0.03%	0.004%
21	5.326	1330	1333	1338	rVV4	610	730	0.03%	0.004%
22	5.423	1360	1363	1367	rVB2	836	671	0.03%	0.004%
23	5.529	1385	1396	1431	rBV	701766	1457268	55.22%	7.782%
24	5.834	1478	1491	1496	rBV10	8233	16740	0.63%	0.089%
25	5.986	1521	1538	1568	rBV	573151	1205889	45.69%	6.440%
26	6.551	1708	1714	1718	rVB4	533	595	0.02%	0.003%
27	6.728	1764	1769	1772	rBV4	1271	1198	0.05%	0.006%
28	6.780	1782	1785	1794	rVB7	1103	1237	0.05%	0.007%
29	6.908	1813	1825	1855	rBV	291805	570977	21.64%	3.049%
30	7.124	1890	1892	1895	rVB3	1287	682	0.03%	0.004%
31	7.175	1905	1908	1911	rVB5	948	646	0.02%	0.003%
32	7.236	1916	1927	1958	rBV	1184461	2098250	79.51%	11.205%
33	7.548	2016	2024	2063	rBV	198097	381859	14.47%	2.039%
34	7.912	2133	2137	2141	rVB3	1097	928	0.04%	0.005%
35	7.934	2141	2144	2147	rBV2	745	570	0.02%	0.003%
36	8.024	2163	2172	2208	rBV2	317634	704559	26.70%	3.762%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037733.D
 Acq On : 04 Oct 2024 09:47
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.397	2286	2288	2292	rVB5	1552	1104	0.04%	0.006%
38	8.461	2302	2308	2312	rBV4	991	954	0.04%	0.005%
39	8.780	2393	2407	2434	rBV	1090381	1813113	68.70%	9.682%
40	9.130	2513	2516	2521	rBV4	1268	860	0.03%	0.005%
41	9.159	2521	2525	2528	rBV4	724	625	0.02%	0.003%
42	9.178	2529	2531	2534	rVB4	1102	604	0.02%	0.003%
43	9.285	2561	2564	2569	rVV5	998	974	0.04%	0.005%
44	9.323	2573	2576	2581	rVB5	914	832	0.03%	0.004%
45	9.410	2597	2603	2604	rBV3	806	635	0.02%	0.003%
46	9.439	2608	2612	2615	rBV2	656	467	0.02%	0.002%
47	9.474	2621	2623	2627	rVB2	841	509	0.02%	0.003%
48	9.493	2627	2629	2631	rBV3	865	513	0.02%	0.003%
49	9.571	2648	2653	2655	rVV2	543	514	0.02%	0.003%
50	9.600	2658	2662	2668	rVB3	786	623	0.02%	0.003%
51	9.629	2668	2671	2674	rBV3	792	715	0.03%	0.004%
52	10.146	2816	2832	2853	rBV	669216	1063265	40.29%	5.678%
53	10.391	2904	2908	2912	rVB5	1031	877	0.03%	0.005%
54	10.420	2912	2917	2919	rBV4	642	577	0.02%	0.003%
55	10.445	2922	2925	2930	rVV3	778	535	0.02%	0.003%
56	10.474	2930	2934	2937	rVV3	1147	908	0.03%	0.005%
57	10.561	2958	2961	2964	rVB2	807	486	0.02%	0.003%
58	10.606	2972	2975	2979	rVB3	832	513	0.02%	0.003%
59	10.661	2986	2992	2995	rBV4	460	510	0.02%	0.003%
60	10.783	3027	3030	3033	rBV3	1303	1040	0.04%	0.006%
61	10.854	3044	3052	3054	rBV3	926	976	0.04%	0.005%
62	10.889	3060	3063	3068	rVB5	952	790	0.03%	0.004%
63	11.133	3133	3139	3141	rBV3	1383	1620	0.06%	0.009%
64	11.178	3141	3153	3192	rVV	1072249	1709635	64.78%	9.130%
65	11.551	3256	3269	3302	rBV	1151659	1867544	70.77%	9.973%
66	11.802	3344	3347	3350	rBV2	926	653	0.02%	0.003%
67	11.821	3350	3353	3356	rBV3	688	599	0.02%	0.003%
68	11.892	3372	3375	3379	rBV4	928	829	0.03%	0.004%
69	12.024	3412	3416	3418	rBV3	775	602	0.02%	0.003%
70	12.413	3535	3537	3544	rVB4	725	830	0.03%	0.004%
71	12.455	3544	3550	3551	rBV4	924	619	0.02%	0.003%
72	12.519	3564	3570	3571	rBV4	567	584	0.02%	0.003%
73	12.590	3588	3592	3598	rVV7	1641	2350	0.09%	0.013%
74	12.622	3601	3602	3607	rVV5	1243	755	0.03%	0.004%
75	12.651	3607	3611	3617	rVB5	573	658	0.02%	0.004%
76	12.763	3638	3646	3649	rBV6	1121	1358	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037733.D
 Acq On : 04 Oct 2024 09:47
 Operator : SY/MD
 Sample : P4239-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.783	3649	3652	3656	rVB3	709	497	0.02%	0.003%
78	12.808	3656	3660	3662	rBV3	690	476	0.02%	0.003%
79	12.850	3669	3673	3676	rBV4	956	762	0.03%	0.004%
80	12.905	3687	3690	3692	rBV2	965	645	0.02%	0.003%
81	12.995	3715	3718	3720	rBV2	1053	598	0.02%	0.003%
82	13.014	3720	3724	3730	rVV3	1046	1155	0.04%	0.006%
83	13.050	3732	3735	3742	rVB6	1107	1020	0.04%	0.005%
84	13.124	3755	3758	3763	rVB4	726	707	0.03%	0.004%
85	13.165	3768	3771	3776	rBV3	1166	747	0.03%	0.004%
86	13.210	3779	3785	3791	rBV5	2622	3621	0.14%	0.019%
87	13.262	3798	3801	3807	rVB4	1032	1012	0.04%	0.005%
88	13.294	3807	3811	3815	rVB4	666	621	0.02%	0.003%
89	13.323	3815	3820	3822	rBV4	916	647	0.02%	0.003%
90	13.387	3834	3840	3842	rBV4	852	861	0.03%	0.005%
91	13.452	3855	3860	3865	rVV5	2837	3808	0.14%	0.020%
92	13.683	3926	3932	3936	rBV9	2397	2806	0.11%	0.015%
93	13.960	4016	4018	4021	rBV4	723	538	0.02%	0.003%
94	13.985	4021	4026	4030	rVB7	1104	1282	0.05%	0.007%
95	14.075	4050	4054	4059	rBV4	965	768	0.03%	0.004%
96	14.127	4067	4070	4074	rBV4	861	720	0.03%	0.004%
97	14.403	4153	4156	4158	rBV3	1183	694	0.03%	0.004%
98	14.808	4279	4282	4286	rVB6	1428	905	0.03%	0.005%
99	15.181	4396	4398	4400	rBV3	1262	591	0.02%	0.003%
100	15.738	4568	4571	4575	rBV6	2009	1819	0.07%	0.010%




Sum of corrected areas: 18726319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037733.D
Acq On : 04 Oct 2024 09:47
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

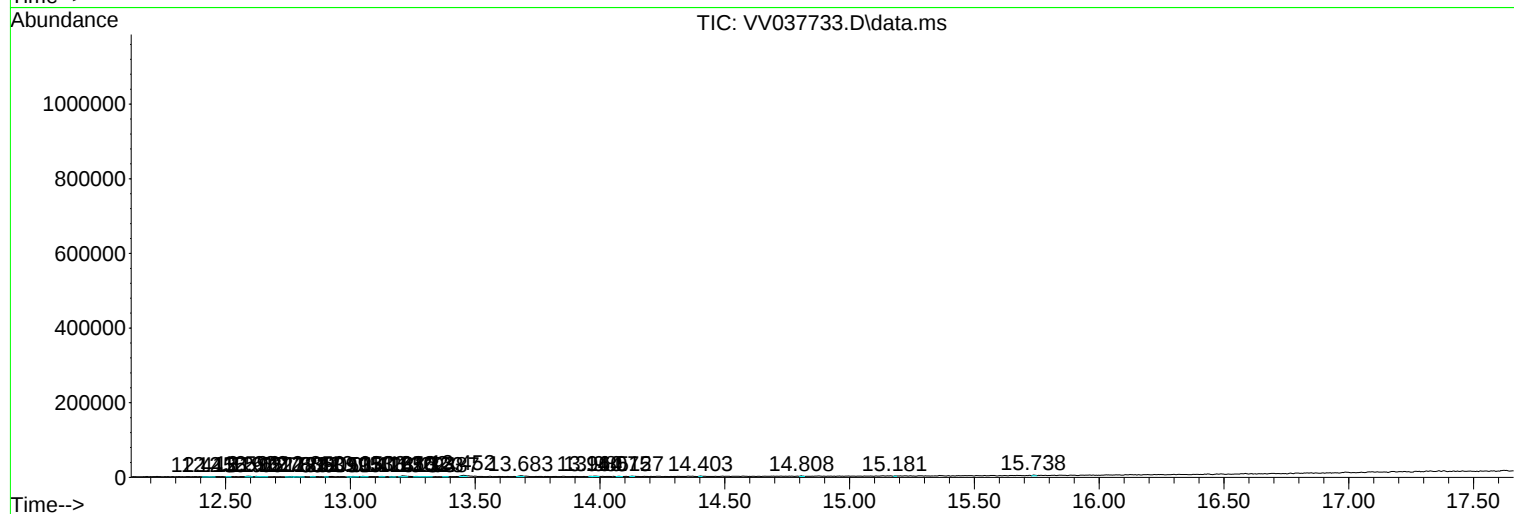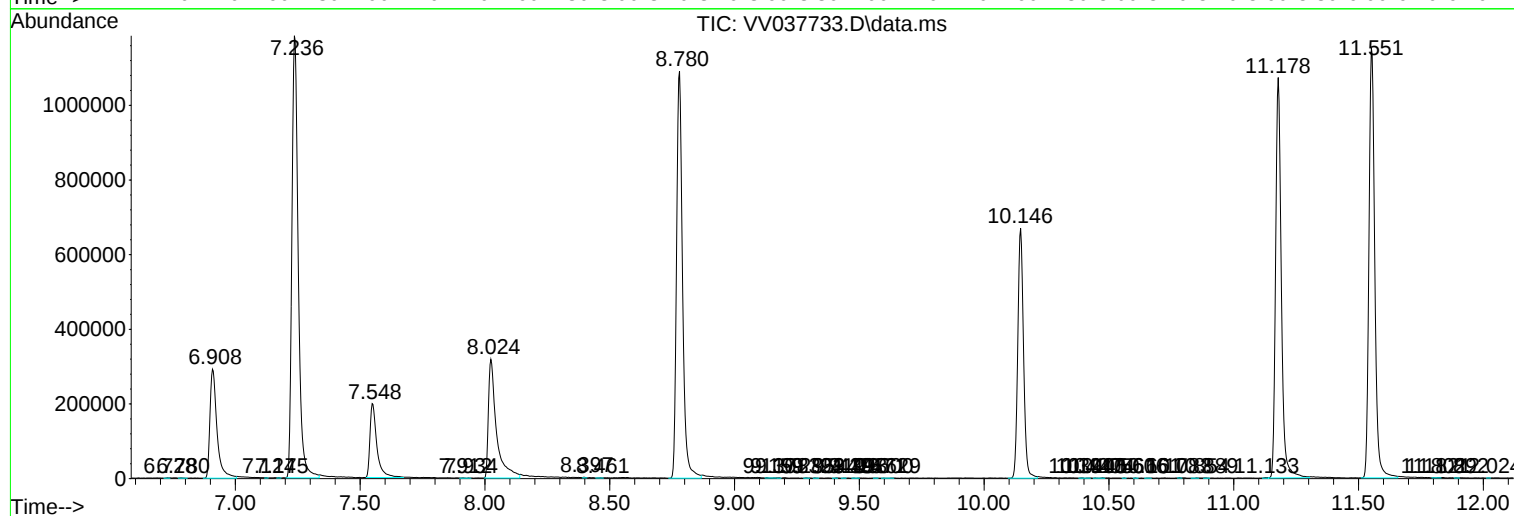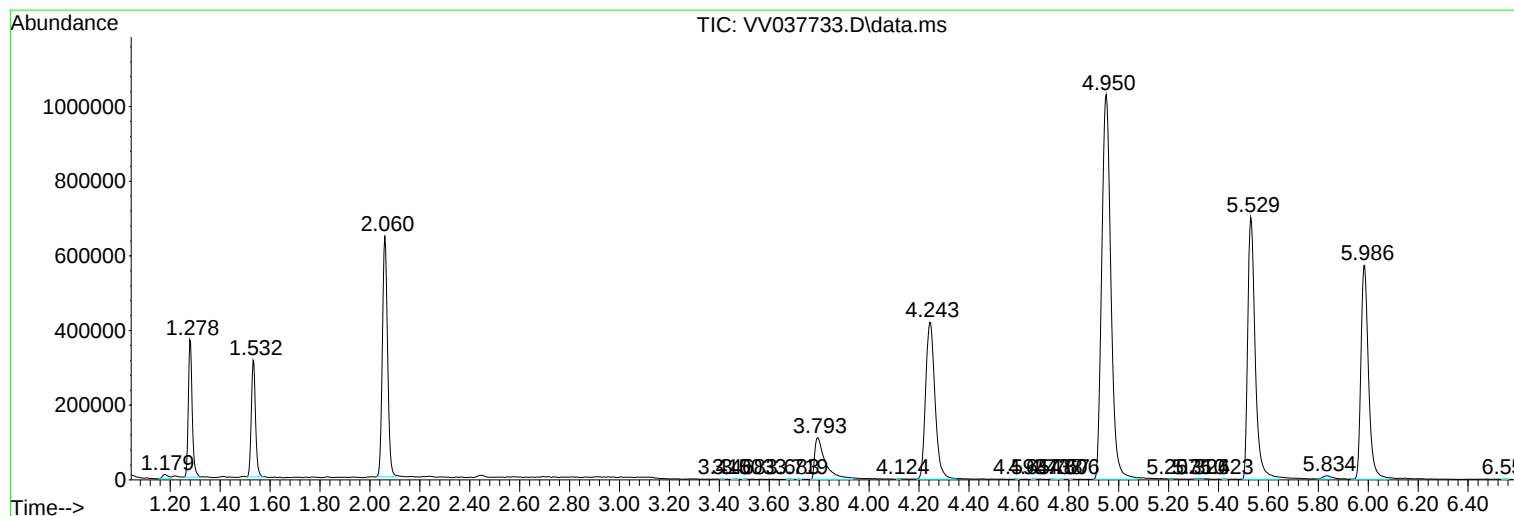

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037733.D
Acq On : 04 Oct 2024 09:47
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037733.D
Acq On : 04 Oct 2024 09:47
Operator : SY/MD
Sample : P4239-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------