

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037740.D
 Acq On : 04 Oct 2024 13:56
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	37	44	51	rBV2	8203	14829	0.65%	0.086%
2	1.278	67	74	88	rBV	286140	314296	13.78%	1.833%
3	1.532	146	153	169	rVB	261482	306523	13.44%	1.787%
4	2.060	307	317	327	rBV	524335	751269	32.94%	4.381%
5	2.114	328	334	351	rVB	58114	96448	4.23%	0.562%
6	3.355	716	720	723	rVB3	797	697	0.03%	0.004%
7	3.375	723	726	728	rBV2	885	500	0.02%	0.003%
8	3.416	737	739	743	rVV4	700	535	0.02%	0.003%
9	3.468	751	755	758	rBV3	716	576	0.03%	0.003%
10	3.545	777	779	783	rBV2	699	552	0.02%	0.003%
11	3.796	848	857	887	rBV	99821	287452	12.60%	1.676%
12	4.105	950	953	957	rVB4	870	659	0.03%	0.004%
13	4.243	978	996	1023	rBV	382367	963556	42.25%	5.619%
14	4.539	1086	1088	1092	rVB5	704	498	0.02%	0.003%
15	4.667	1123	1128	1130	rBV3	661	645	0.03%	0.004%
16	4.780	1159	1163	1167	rVB3	711	637	0.03%	0.004%
17	4.950	1199	1216	1248	rBV2	890271	2280697	100.00%	13.300%
18	5.326	1331	1333	1337	rVB4	1120	660	0.03%	0.004%
19	5.455	1370	1373	1377	rBV3	903	589	0.03%	0.003%
20	5.529	1385	1396	1438	rBV	711823	1483794	65.06%	8.653%
21	5.715	1452	1454	1456	rBV2	1419	609	0.03%	0.004%
22	5.825	1481	1488	1491	rBV2	10110	13015	0.57%	0.076%
23	5.982	1524	1537	1568	rBV	508835	1060643	46.51%	6.185%
24	6.137	1582	1585	1587	rBV3	1442	969	0.04%	0.006%
25	6.220	1607	1611	1613	rBV4	656	568	0.02%	0.003%
26	6.375	1657	1659	1664	rVB5	659	550	0.02%	0.003%
27	6.465	1684	1687	1691	rVB5	679	509	0.02%	0.003%
28	6.526	1703	1706	1709	rVB3	869	504	0.02%	0.003%
29	6.574	1715	1721	1726	rVB4	755	848	0.04%	0.005%
30	6.657	1744	1747	1751	rBV3	957	767	0.03%	0.004%
31	6.908	1815	1825	1855	rBV	253672	502319	22.02%	2.929%
32	7.153	1897	1901	1905	rVB5	889	744	0.03%	0.004%
33	7.178	1905	1909	1911	rBV5	706	568	0.02%	0.003%
34	7.236	1916	1927	1953	rBV	985154	1759085	77.13%	10.258%
35	7.551	2016	2025	2048	rBV	171336	320401	14.05%	1.868%
36	7.847	2114	2117	2123	rBV6	1448	1228	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037740.D
 Acq On : 04 Oct 2024 13:56
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.873	2123	2125	2130	rVB5	906	623	0.03%	0.004%
38	7.982	2155	2159	2163	rVB7	764	658	0.03%	0.004%
39	8.024	2163	2172	2218	rBV2	291723	663330	29.08%	3.868%
40	8.317	2261	2263	2269	rBV6	1002	989	0.04%	0.006%
41	8.436	2295	2300	2303	rBV7	1384	1464	0.06%	0.009%
42	8.648	2360	2366	2367	rBV4	1816	1432	0.06%	0.008%
43	8.776	2391	2406	2439	rBV	1113736	1867995	81.90%	10.893%
44	9.034	2483	2486	2489	rBV3	868	779	0.03%	0.005%
45	9.114	2508	2511	2516	rBV4	1058	943	0.04%	0.005%
46	9.153	2517	2523	2524	rBV4	661	548	0.02%	0.003%
47	9.284	2560	2564	2566	rBV4	857	671	0.03%	0.004%
48	9.358	2584	2587	2591	rBV3	742	689	0.03%	0.004%
49	9.497	2625	2630	2633	rBV5	1062	975	0.04%	0.006%
50	9.709	2687	2696	2697	rBV6	3114	2734	0.12%	0.016%
51	9.786	2717	2720	2724	rVB4	1129	781	0.03%	0.005%
52	9.818	2724	2730	2735	rBV4	1153	1486	0.07%	0.009%
53	9.882	2742	2750	2762	rBV9	6830	11744	0.51%	0.068%
54	10.098	2813	2817	2819	rBV4	680	492	0.02%	0.003%
55	10.146	2820	2832	2851	rBV	591806	934222	40.96%	5.448%
56	10.384	2902	2906	2908	rVV2	622	518	0.02%	0.003%
57	10.474	2931	2934	2938	rVB4	888	575	0.03%	0.003%
58	10.558	2957	2960	2962	rBV3	1262	825	0.04%	0.005%
59	10.622	2976	2980	2981	rBV4	1131	704	0.03%	0.004%
60	10.873	3052	3058	3061	rVB4	579	616	0.03%	0.004%
61	10.921	3070	3073	3077	rBV4	799	634	0.03%	0.004%
62	10.992	3091	3095	3102	rVB9	2012	2335	0.10%	0.014%
63	11.030	3103	3107	3114	rVB5	983	1065	0.05%	0.006%
64	11.069	3115	3119	3121	rBV3	819	582	0.03%	0.003%
65	11.124	3127	3136	3142	rBV8	7590	12422	0.54%	0.072%
66	11.178	3142	3153	3183	rBV	1081909	1730881	75.89%	10.093%
67	11.468	3238	3243	3245	rBV5	1168	1057	0.05%	0.006%
68	11.551	3248	3269	3297	rVV	1047911	1688071	74.02%	9.844%
69	11.834	3353	3357	3360	rBV5	1694	1476	0.06%	0.009%
70	11.956	3384	3395	3400	rBV10	3913	6262	0.27%	0.037%
71	12.085	3431	3435	3438	rVB6	971	689	0.03%	0.004%
72	12.127	3443	3448	3449	rBV3	1110	845	0.04%	0.005%
73	12.188	3464	3467	3471	rVB4	1302	824	0.04%	0.005%
74	12.252	3482	3487	3488	rBV3	1781	1093	0.05%	0.006%
75	12.387	3526	3529	3534	rBV5	1043	891	0.04%	0.005%
76	12.445	3543	3547	3549	rVV2	867	616	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037740.D
 Acq On : 04 Oct 2024 13:56
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.506	3563	3566	3569	rVV5	1066	670	0.03%	0.004%
78	12.525	3570	3572	3575	rVV	1266	721	0.03%	0.004%
79	12.767	3645	3647	3650	rVB3	1143	566	0.02%	0.003%
80	12.786	3650	3653	3658	rBV3	889	1008	0.04%	0.006%
81	13.095	3747	3749	3755	rVB6	1529	1102	0.05%	0.006%
82	13.178	3772	3775	3778	rBV3	761	601	0.03%	0.004%
83	13.210	3783	3785	3787	rBV3	1261	723	0.03%	0.004%
84	13.458	3859	3862	3865	rBV3	1215	925	0.04%	0.005%
85	13.477	3865	3868	3873	rVV6	1613	1552	0.07%	0.009%
86	13.567	3893	3896	3900	rVB4	926	722	0.03%	0.004%
87	13.596	3900	3905	3906	rBV3	906	644	0.03%	0.004%
88	13.689	3931	3934	3939	rBV4	932	592	0.03%	0.003%
89	13.789	3963	3965	3968	rBV2	641	517	0.02%	0.003%
90	13.805	3968	3970	3974	rVV3	1016	594	0.03%	0.003%
91	13.882	3988	3994	3997	rBV4	863	991	0.04%	0.006%
92	14.037	4038	4042	4044	rBV4	939	877	0.04%	0.005%
93	14.345	4133	4138	4140	rBV5	2247	2216	0.10%	0.013%
94	14.439	4164	4167	4169	rBV3	1052	654	0.03%	0.004%
95	14.805	4278	4281	4282	rBV4	1045	507	0.02%	0.003%
96	14.947	4323	4325	4327	rBV2	1113	603	0.03%	0.004%
97	15.011	4342	4345	4349	rBV6	1193	1087	0.05%	0.006%
98	15.053	4350	4358	4366	rVV9	7873	13548	0.59%	0.079%
99	15.127	4378	4381	4383	rBV5	1067	583	0.03%	0.003%
100	15.548	4509	4512	4518	rBV5	2427	2364	0.10%	0.014%




Sum of corrected areas: 17148642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037740.D
Acq On : 04 Oct 2024 13:56
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

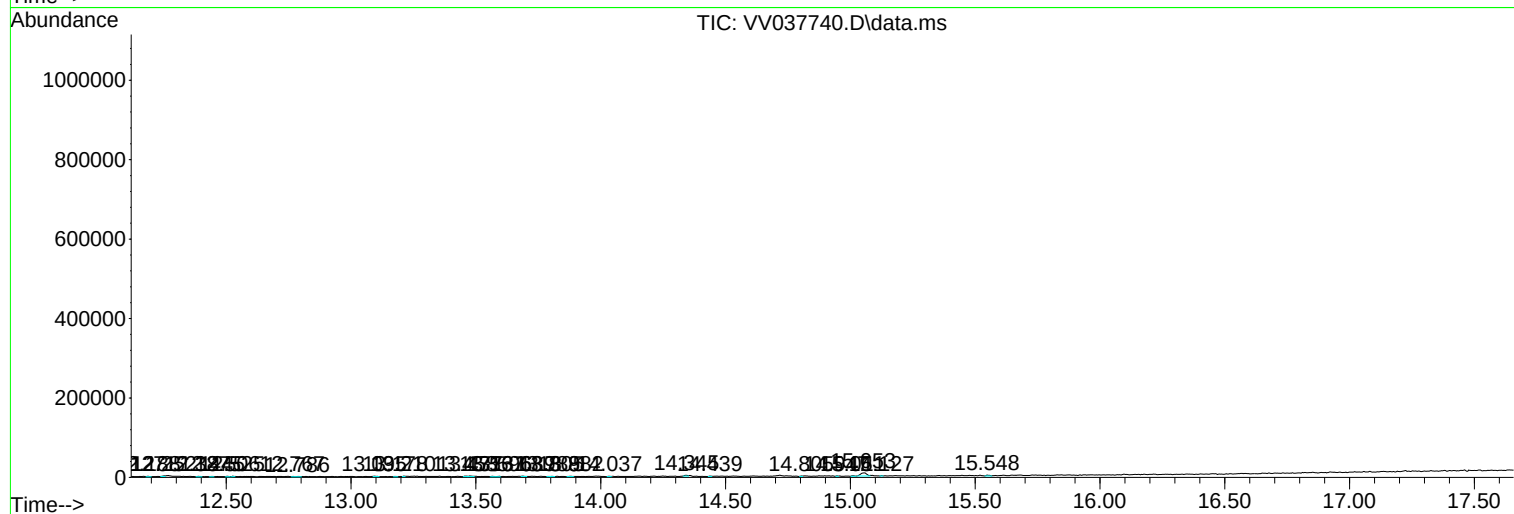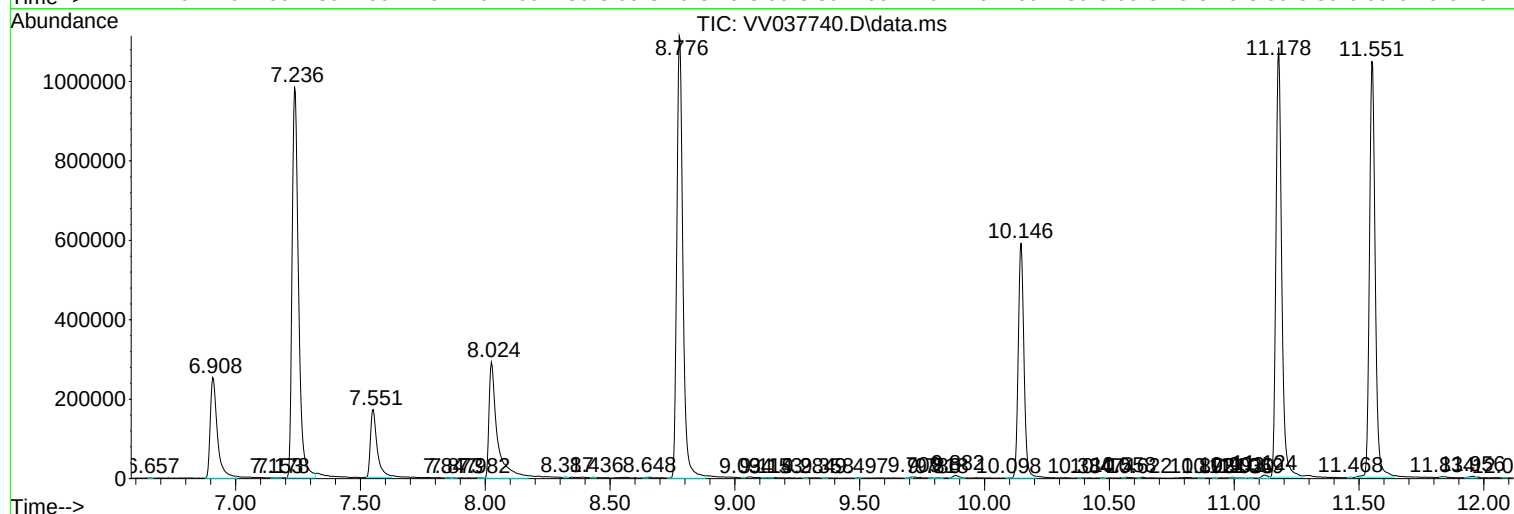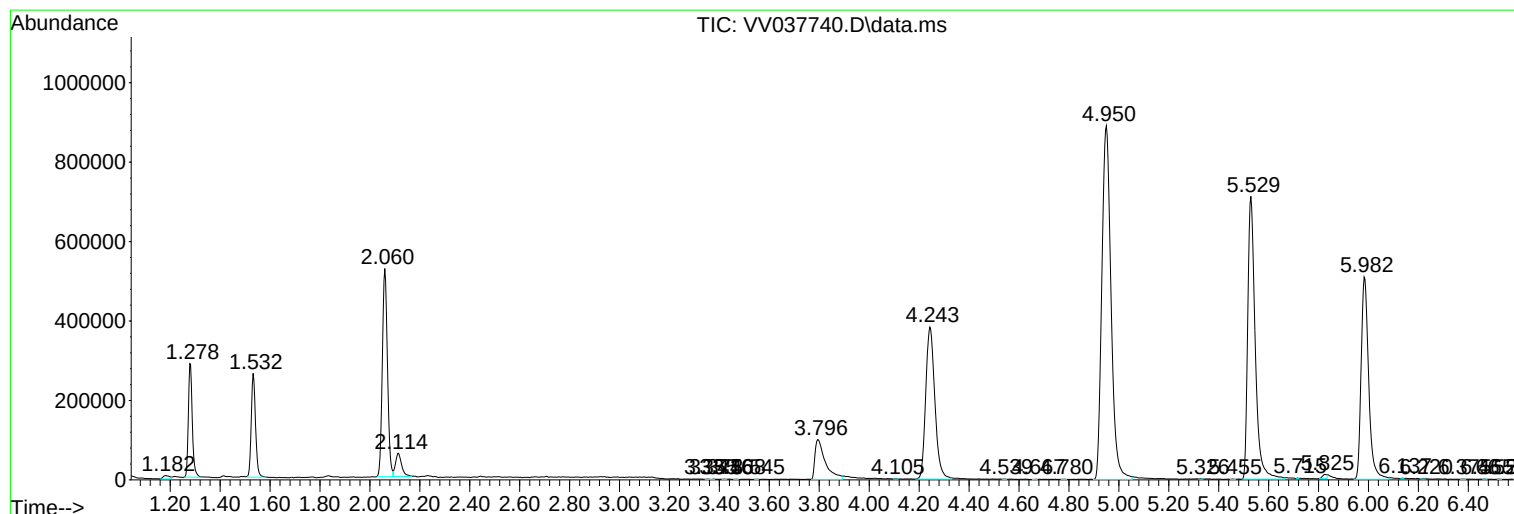

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037740.D
Acq On : 04 Oct 2024 13:56
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037740.D
Acq On : 04 Oct 2024 13:56
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------