

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037741.D
 Acq On : 04 Oct 2024 14:45
 Operator : SY/MD
 Sample : P4284-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	292951	315513	13.66%	1.859%
2	1.532	146	153	167	rVB	271517	306764	13.28%	1.808%
3	2.056	307	316	327	rBV	533074	772377	33.43%	4.551%
4	3.285	695	698	700	rBV3	934	597	0.03%	0.004%
5	3.410	735	737	739	rBV2	599	278	0.01%	0.002%
6	3.516	768	770	771	rBV2	331	111	0.00%	0.001%
7	3.635	805	807	810	rBV3	573	399	0.02%	0.002%
8	3.664	814	816	818	rVB3	324	109	0.00%	0.001%
9	3.683	820	822	823	rVV	530	165	0.01%	0.001%
10	3.706	827	829	830	rBV	564	260	0.01%	0.002%
11	3.789	846	855	886	rBV	94886	276118	11.95%	1.627%
12	4.240	980	995	1030	rVB	378169	960773	41.59%	5.661%
13	4.510	1077	1079	1081	rBV2	566	212	0.01%	0.001%
14	4.532	1084	1086	1090	rVB4	612	308	0.01%	0.002%
15	4.555	1090	1093	1095	rBV4	754	451	0.02%	0.003%
16	4.571	1096	1098	1102	rVB3	802	471	0.02%	0.003%
17	4.593	1102	1105	1109	rBV4	801	533	0.02%	0.003%
18	4.609	1109	1110	1117	rVB5	740	545	0.02%	0.003%
19	4.638	1117	1119	1121	rBV2	449	250	0.01%	0.001%
20	4.690	1131	1135	1136	rBV	527	322	0.01%	0.002%
21	4.741	1148	1151	1156	rVB4	650	508	0.02%	0.003%
22	4.776	1156	1162	1165	rBV2	414	434	0.02%	0.003%
23	4.802	1167	1170	1174	rVB4	809	591	0.03%	0.003%
24	4.841	1180	1182	1183	rBV	280	113	0.00%	0.001%
25	4.850	1183	1185	1190	rVB3	765	385	0.02%	0.002%
26	4.947	1190	1215	1250	rBV2	904214	2310343	100.00%	13.614%
27	5.426	1361	1364	1366	rBV	591	342	0.01%	0.002%
28	5.468	1372	1377	1379	rBV4	864	719	0.03%	0.004%
29	5.481	1379	1381	1382	rBV3	782	300	0.01%	0.002%
30	5.526	1384	1395	1423	rBV	717601	1485550	64.30%	8.754%
31	5.825	1479	1488	1490	rBV6	10242	14154	0.61%	0.083%
32	5.979	1524	1536	1573	rBV	517072	1074500	46.51%	6.332%
33	6.317	1636	1641	1646	rBV6	1308	1718	0.07%	0.010%
34	6.413	1669	1671	1673	rBV2	651	375	0.02%	0.002%
35	6.513	1699	1702	1704	rBV4	753	251	0.01%	0.001%
36	6.567	1717	1719	1720	rBV	69	16	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037741.D
 Acq On : 04 Oct 2024 14:45
 Operator : SY/MD
 Sample : P4284-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.583	1720	1724	1725	rBV3	472	364	0.02%	0.002%
38	6.600	1727	1729	1731	rVV4	532	271	0.01%	0.002%
39	6.609	1731	1732	1734	rVB2	693	151	0.01%	0.001%
40	6.628	1734	1738	1739	rBV2	456	243	0.01%	0.001%
41	6.680	1751	1754	1756	rBV3	659	494	0.02%	0.003%
42	6.715	1763	1765	1766	rBV2	378	181	0.01%	0.001%
43	6.744	1771	1774	1775	rBV	294	147	0.01%	0.001%
44	6.757	1776	1778	1781	rVV2	595	269	0.01%	0.002%
45	6.773	1781	1783	1785	rVV3	564	353	0.02%	0.002%
46	6.796	1788	1790	1795	rBV3	457	336	0.01%	0.002%
47	6.834	1800	1802	1804	rVB2	457	224	0.01%	0.001%
48	6.847	1804	1806	1808	rBV2	131	71	0.00%	0.000%
49	6.857	1808	1809	1812	rVB2	398	121	0.01%	0.001%
50	6.905	1812	1824	1848	rBV	252701	494118	21.39%	2.912%
51	7.236	1916	1927	1952	rBV	983874	1754538	75.94%	10.339%
52	7.548	2015	2024	2052	rBV	171836	326863	14.15%	1.926%
53	8.024	2163	2172	2211	rBV2	265435	613141	26.54%	3.613%
54	8.616	2354	2356	2358	rVB2	1048	471	0.02%	0.003%
55	8.644	2358	2365	2372	rBV2	1626	2777	0.12%	0.016%
56	8.722	2387	2389	2392	rBV4	532	361	0.02%	0.002%
57	8.776	2395	2406	2442	rBV	1131554	1882300	81.47%	11.092%
58	9.349	2581	2584	2586	rBV3	940	729	0.03%	0.004%
59	9.445	2613	2614	2616	rBV2	452	221	0.01%	0.001%
60	9.532	2639	2641	2644	rBV2	770	336	0.01%	0.002%
61	9.564	2648	2651	2653	rBV	666	480	0.02%	0.003%
62	9.577	2653	2655	2657	rBV4	792	445	0.02%	0.003%
63	9.641	2668	2675	2679	rBV6	1195	1589	0.07%	0.009%
64	9.718	2690	2699	2705	rBV7	3102	4922	0.21%	0.029%
65	9.767	2711	2714	2715	rBV	599	308	0.01%	0.002%
66	9.779	2715	2718	2719	rVV	744	381	0.02%	0.002%
67	9.882	2745	2750	2752	rBV4	4316	3894	0.17%	0.023%
68	10.056	2802	2804	2806	rBV2	498	293	0.01%	0.002%
69	10.146	2821	2832	2848	rBV	578319	912952	39.52%	5.380%
70	10.304	2879	2881	2883	rBV3	649	342	0.01%	0.002%
71	10.451	2923	2927	2929	rBV4	575	538	0.02%	0.003%
72	10.506	2942	2944	2947	rBV2	536	271	0.01%	0.002%
73	10.564	2954	2962	2968	rBV9	2914	4130	0.18%	0.024%
74	10.760	3020	3023	3025	rBV3	790	441	0.02%	0.003%
75	10.860	3051	3054	3056	rBV	653	444	0.02%	0.003%
76	10.898	3063	3066	3068	rBV2	680	427	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037741.D
Acq On : 04 Oct 2024 14:45
Operator : SY/MD
Sample : P4284-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	10.995	3090	3096	3100	rVB7	1892	1806	0.08%	0.011%
78	11.120	3126	3135	3142	rBV7	9699	15279	0.66%	0.090%
79	11.178	3142	3153	3181	rVV	1104371	1744658	75.52%	10.280%
80	11.551	3259	3269	3299	rVB	1033968	1662171	71.94%	9.794%
81	11.947	3384	3392	3396	rBV9	4251	6311	0.27%	0.037%
82	13.059	3736	3738	3741	rVB4	1063	602	0.03%	0.004%
83	13.374	3828	3836	3839	rBV7	1433	1971	0.09%	0.012%




Sum of corrected areas: 16970590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037741.D
Acq On : 04 Oct 2024 14:45
Operator : SY/MD
Sample : P4284-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

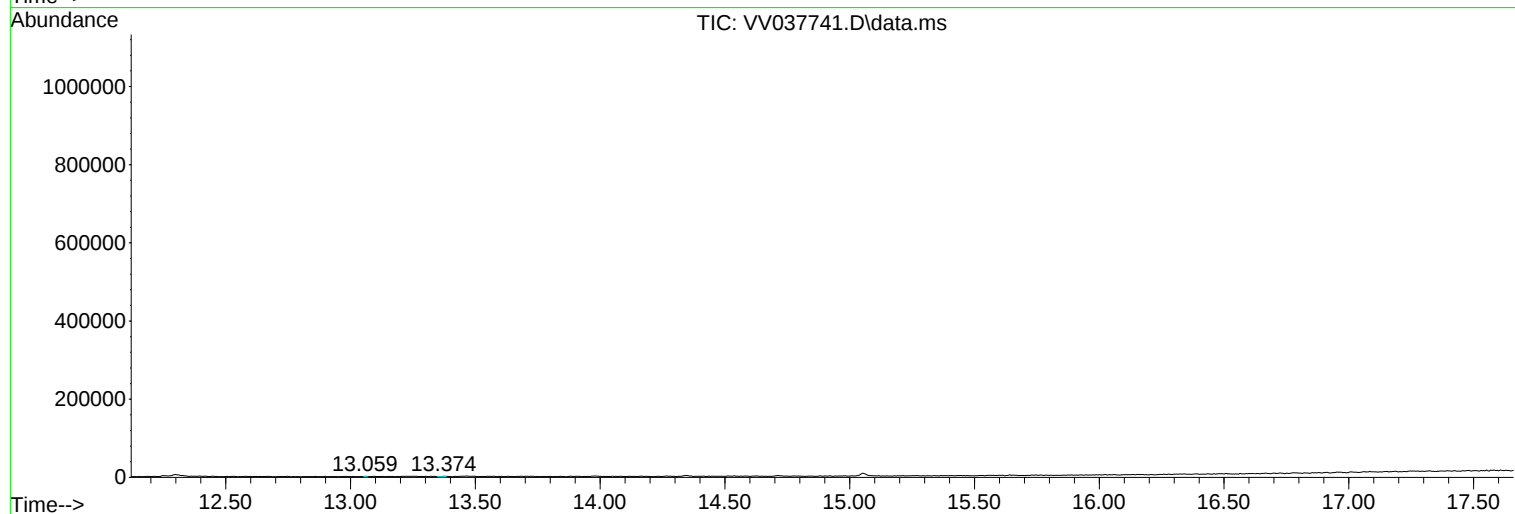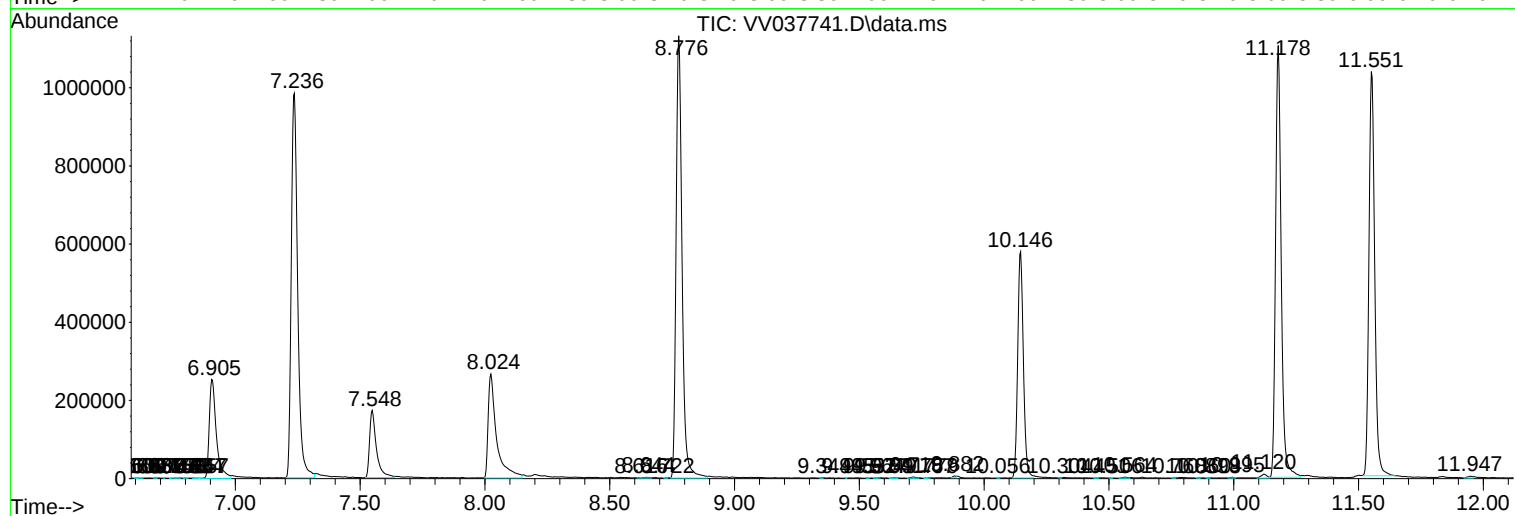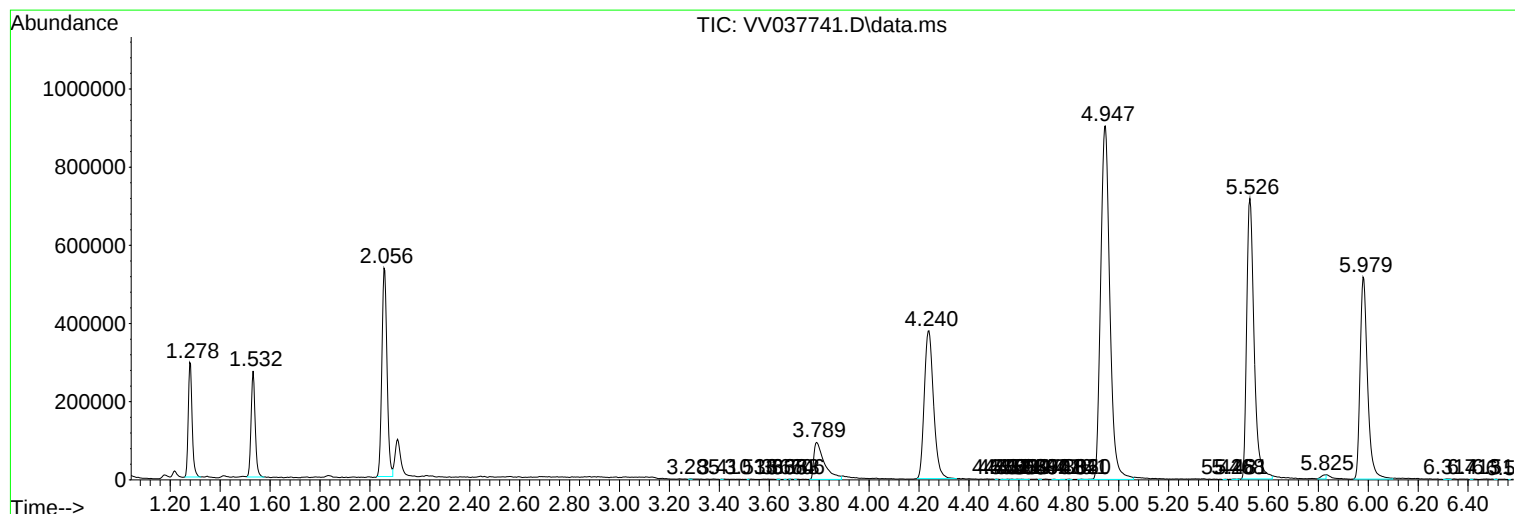

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037741.D
Acq On : 04 Oct 2024 14:45
Operator : SY/MD
Sample : P4284-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037741.D
Acq On : 04 Oct 2024 14:45
Operator : SY/MD
Sample : P4284-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
