

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037742.D
 Acq On : 04 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	38	44	51	rBV2	6064	10989	0.49%	0.066%
2	1.278	68	74	88	rVB	273482	296273	13.34%	1.790%
3	1.532	146	153	170	rVB	260203	300484	13.53%	1.816%
4	2.060	308	317	327	rBV	504144	722638	32.53%	4.366%
5	3.310	704	706	709	rBV2	896	641	0.03%	0.004%
6	3.664	814	816	818	rVB2	279	94	0.00%	0.001%
7	3.674	818	819	820	rBV	270	93	0.00%	0.001%
8	3.709	828	830	836	rVB3	472	405	0.02%	0.002%
9	3.738	836	839	841	rBV2	304	163	0.01%	0.001%
10	3.751	841	843	844	rBV2	358	127	0.01%	0.001%
11	3.760	844	846	848	rVB2	390	146	0.01%	0.001%
12	3.796	848	857	895	rBV	101816	298695	13.45%	1.805%
13	4.243	982	996	1026	rVB	367962	931468	41.93%	5.628%
14	4.519	1078	1082	1088	rVB4	778	704	0.03%	0.004%
15	4.584	1099	1102	1105	rBV4	799	467	0.02%	0.003%
16	4.638	1116	1119	1120	rBV2	416	277	0.01%	0.002%
17	4.725	1144	1146	1147	rBV2	535	218	0.01%	0.001%
18	4.764	1153	1158	1159	rBV2	636	402	0.02%	0.002%
19	4.805	1168	1171	1172	rBV	440	224	0.01%	0.001%
20	4.841	1178	1182	1187	rBV3	611	577	0.03%	0.003%
21	4.876	1191	1193	1196	rVB2	572	211	0.01%	0.001%
22	4.950	1200	1216	1247	rBV2	875772	2221366	100.00%	13.422%
23	5.452	1368	1372	1374	rBV3	674	476	0.02%	0.003%
24	5.468	1374	1377	1378	rBV2	428	195	0.01%	0.001%
25	5.477	1378	1380	1382	rBV2	577	266	0.01%	0.002%
26	5.529	1385	1396	1430	rBV	688693	1427423	64.26%	8.625%
27	5.985	1525	1538	1568	rBV	497353	1040373	46.83%	6.286%
28	6.288	1629	1632	1633	rBV2	903	484	0.02%	0.003%
29	6.371	1653	1658	1662	rVB5	1226	987	0.04%	0.006%
30	6.397	1662	1666	1671	rBV7	658	801	0.04%	0.005%
31	6.474	1688	1690	1695	rBV4	978	639	0.03%	0.004%
32	6.493	1695	1696	1698	rVB	779	235	0.01%	0.001%
33	6.506	1698	1700	1701	rBV2	708	276	0.01%	0.002%
34	6.551	1712	1714	1716	rBV	444	216	0.01%	0.001%
35	6.561	1716	1717	1721	rVB3	715	431	0.02%	0.003%
36	6.577	1721	1722	1723	rBV3	644	235	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037742.D
 Acq On : 04 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4284-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.600	1727	1729	1730	rVB	288	65	0.00%	0.000%
38	6.616	1731	1734	1736	rBV3	627	353	0.02%	0.002%
39	6.648	1742	1744	1746	rBV3	557	242	0.01%	0.001%
40	6.680	1751	1754	1756	rBV3	854	533	0.02%	0.003%
41	6.735	1768	1771	1773	rBV2	858	498	0.02%	0.003%
42	6.818	1795	1797	1798	rBV	201	58	0.00%	0.000%
43	6.854	1804	1808	1809	rBV2	654	441	0.02%	0.003%
44	6.908	1815	1825	1854	rBV	248888	484265	21.80%	2.926%
45	7.239	1917	1928	1969	rBV	958800	1725125	77.66%	10.424%
46	7.551	2016	2025	2049	rBV	170081	320081	14.41%	1.934%
47	7.918	2137	2139	2141	rBV2	658	339	0.02%	0.002%
48	7.950	2147	2149	2153	rVB2	680	430	0.02%	0.003%
49	8.024	2164	2172	2221	rBV2	286095	666763	30.02%	4.029%
50	8.780	2396	2407	2431	rBV	1087531	1802419	81.14%	10.891%
51	9.243	2549	2551	2553	rBV3	603	358	0.02%	0.002%
52	9.281	2561	2563	2564	rBV	814	364	0.02%	0.002%
53	9.342	2580	2582	2586	rVB3	725	268	0.01%	0.002%
54	9.529	2637	2640	2642	rBV3	723	432	0.02%	0.003%
55	9.567	2648	2652	2654	rBV3	456	307	0.01%	0.002%
56	9.580	2654	2656	2657	rBV	658	246	0.01%	0.001%
57	9.622	2667	2669	2671	rVB2	306	122	0.01%	0.001%
58	9.635	2671	2673	2678	rVB5	866	423	0.02%	0.003%
59	9.667	2679	2683	2684	rBV3	765	431	0.02%	0.003%
60	9.712	2691	2697	2702	rBV6	2982	4046	0.18%	0.024%
61	9.776	2715	2717	2720	rVB2	554	260	0.01%	0.002%
62	9.799	2722	2724	2725	rBV	610	226	0.01%	0.001%
63	9.889	2746	2752	2765	rVB9	6396	10045	0.45%	0.061%
64	9.963	2772	2775	2776	rBV2	457	264	0.01%	0.002%
65	10.046	2798	2801	2803	rVB	564	272	0.01%	0.002%
66	10.056	2803	2804	2805	rBV	219	52	0.00%	0.000%
67	10.066	2805	2807	2808	rBV	275	95	0.00%	0.001%
68	10.085	2808	2813	2814	rBV2	676	527	0.02%	0.003%
69	10.146	2821	2832	2848	rBV	590461	920143	41.42%	5.560%
70	10.294	2876	2878	2879	rBV	914	389	0.02%	0.002%
71	10.635	2979	2984	2991	rVB7	2010	2423	0.11%	0.015%
72	10.712	3006	3008	3012	rBV3	620	511	0.02%	0.003%
73	10.750	3018	3020	3021	rBV2	573	185	0.01%	0.001%
74	10.892	3063	3064	3067	rBV2	235	129	0.01%	0.001%
75	10.924	3072	3074	3075	rBV	561	298	0.01%	0.002%
76	10.985	3088	3093	3094	rBV4	1697	1305	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037742.D
Acq On : 04 Oct 2024 15:06
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	11.075	3118	3121	3128	rBV5	780	1089	0.05%	0.007%
78	11.123	3128	3136	3142	rBV5	10423	14656	0.66%	0.089%
79	11.178	3143	3153	3183	rVV	1063358	1689805	76.07%	10.210%
80	11.551	3259	3269	3299	rVB	1009809	1634498	73.58%	9.876%
81	12.432	3541	3543	3546	rBV2	1174	821	0.04%	0.005%
82	12.721	3631	3633	3638	rVB4	749	640	0.03%	0.004%
83	12.898	3685	3688	3692	rBV3	767	764	0.03%	0.005%
84	12.934	3696	3699	3702	rBV3	1340	831	0.04%	0.005%
85	13.229	3789	3791	3792	rBV2	1052	502	0.02%	0.003%
86	13.406	3841	3846	3848	rBV4	1082	1104	0.05%	0.007%




Sum of corrected areas: 16550142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037742.D
Acq On : 04 Oct 2024 15:06
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

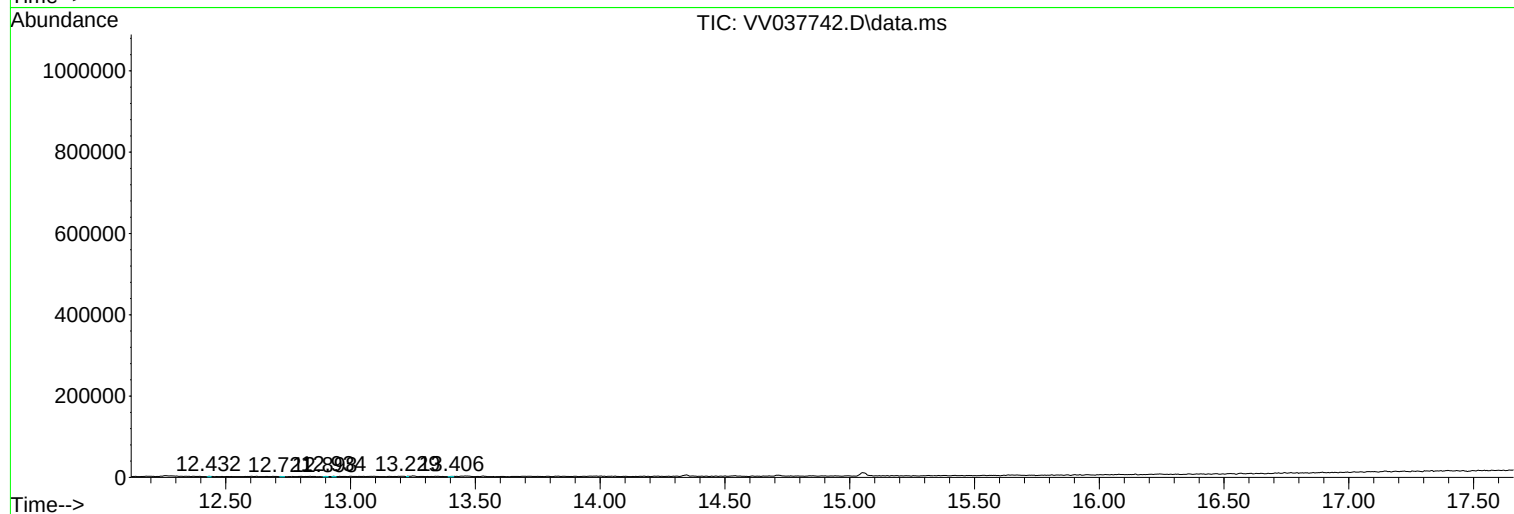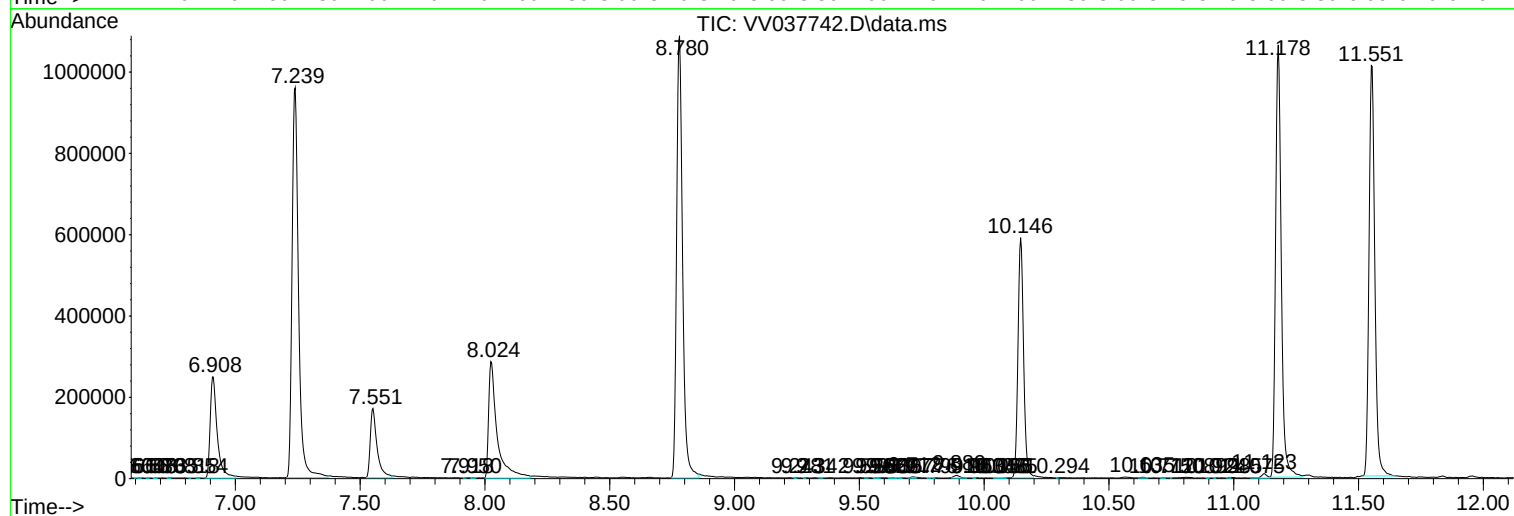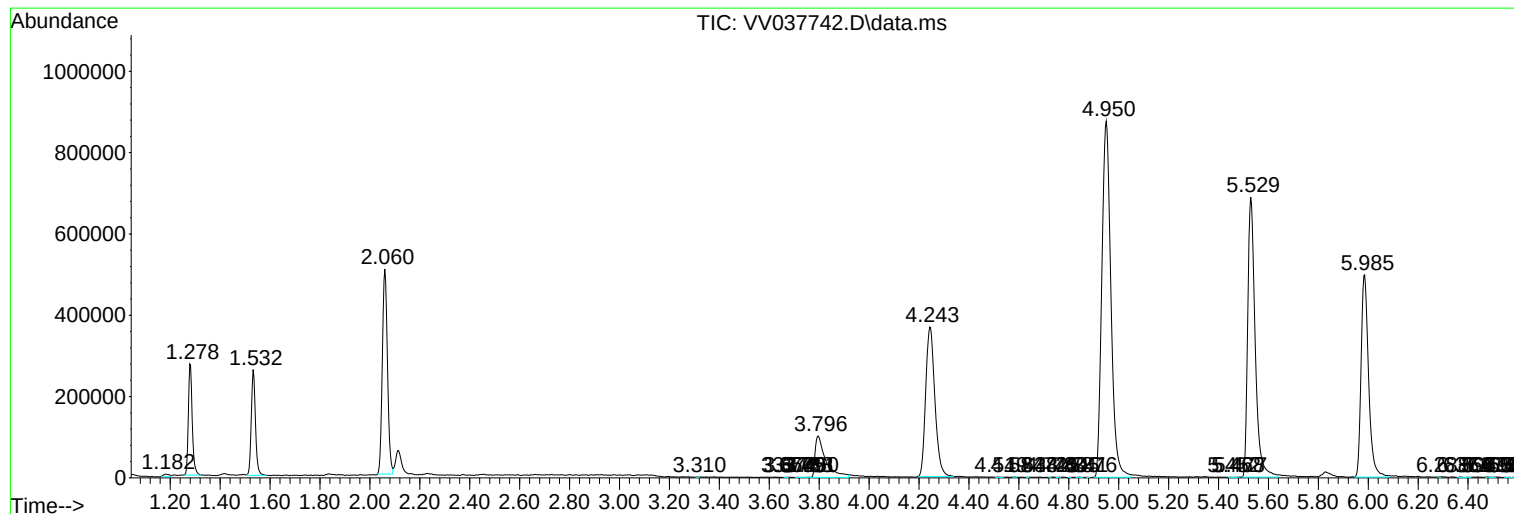

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037742.D
Acq On : 04 Oct 2024 15:06
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037742.D
Acq On : 04 Oct 2024 15:06
Operator : SY/MD
Sample : P4284-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------