

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037743.D
 Acq On : 04 Oct 2024 15:27
 Operator : SY/MD
 Sample : P4284-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	367926	397400	15.14%	2.160%
2	1.532	146	153	169	rVB	313830	368909	14.05%	2.005%
3	2.060	307	317	343	rVB	649801	933162	35.55%	5.073%
4	3.294	699	701	705	rVB3	898	499	0.02%	0.003%
5	3.436	743	745	748	rBV	648	332	0.01%	0.002%
6	3.452	748	750	751	rBV	478	180	0.01%	0.001%
7	3.474	755	757	759	rBV2	352	151	0.01%	0.001%
8	3.487	759	761	762	rBV	429	155	0.01%	0.001%
9	3.519	769	771	773	rBV2	523	304	0.01%	0.002%
10	3.561	778	784	786	rBV2	853	851	0.03%	0.005%
11	3.597	792	795	797	rBV3	501	256	0.01%	0.001%
12	3.609	797	799	802	rVB2	558	230	0.01%	0.001%
13	3.632	804	806	808	rBV	358	172	0.01%	0.001%
14	3.654	811	813	814	rBV	249	135	0.01%	0.001%
15	3.696	824	826	829	rBV4	465	258	0.01%	0.001%
16	3.764	842	847	849	rBV3	748	567	0.02%	0.003%
17	3.796	849	857	887	rBV	109878	311574	11.87%	1.694%
18	4.143	962	965	966	rBV2	902	484	0.02%	0.003%
19	4.243	978	996	1027	rBV	428945	1086750	41.40%	5.908%
20	4.558	1092	1094	1095	rBV	378	106	0.00%	0.001%
21	4.622	1112	1114	1115	rVB2	738	210	0.01%	0.001%
22	4.638	1115	1119	1121	rBV2	447	286	0.01%	0.002%
23	4.654	1122	1124	1128	rVB2	637	399	0.02%	0.002%
24	4.687	1132	1134	1136	rBV2	306	138	0.01%	0.001%
25	4.709	1139	1141	1143	rBV2	674	376	0.01%	0.002%
26	4.767	1156	1159	1161	rBV3	279	204	0.01%	0.001%
27	4.822	1174	1176	1179	rVB3	643	350	0.01%	0.002%
28	4.841	1179	1182	1183	rBV	404	215	0.01%	0.001%
29	4.896	1196	1199	1200	rBV	536	312	0.01%	0.002%
30	4.950	1200	1216	1256	rVV2	1026388	2624777	100.00%	14.269%
31	5.317	1327	1330	1332	rBV2	1210	754	0.03%	0.004%
32	5.407	1354	1358	1362	rBV5	965	774	0.03%	0.004%
33	5.426	1362	1364	1368	rVB3	421	297	0.01%	0.002%
34	5.468	1376	1377	1379	rBV2	412	173	0.01%	0.001%
35	5.529	1385	1396	1434	rBV	675104	1404422	53.51%	7.635%
36	5.986	1525	1538	1565	rBV	577944	1196072	45.57%	6.502%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037743.D
 Acq On : 04 Oct 2024 15:27
 Operator : SY/MD
 Sample : P4284-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.336	1643	1647	1648	rBV	557	354	0.01%	0.002%
38	6.365	1653	1656	1659	rBV4	794	379	0.01%	0.002%
39	6.381	1659	1661	1669	rVB6	695	811	0.03%	0.004%
40	6.420	1669	1673	1674	rBV3	737	514	0.02%	0.003%
41	6.452	1681	1683	1688	rVB3	600	298	0.01%	0.002%
42	6.584	1719	1724	1725	rBV5	654	525	0.02%	0.003%
43	6.612	1731	1733	1735	rVB	548	222	0.01%	0.001%
44	6.632	1735	1739	1740	rBV2	250	133	0.01%	0.001%
45	6.661	1745	1748	1750	rBV3	491	361	0.01%	0.002%
46	6.706	1760	1762	1768	rVB4	537	528	0.02%	0.003%
47	6.735	1768	1771	1774	rBV3	879	659	0.03%	0.004%
48	6.802	1790	1792	1795	rVB4	549	284	0.01%	0.002%
49	6.815	1795	1796	1800	rVB	528	187	0.01%	0.001%
50	6.850	1805	1807	1809	rBV2	381	240	0.01%	0.001%
51	6.870	1809	1813	1815	rBV2	566	487	0.02%	0.003%
52	6.908	1815	1825	1851	rBV	293378	563438	21.47%	3.063%
53	7.236	1916	1927	1957	rBV	1159715	2062223	78.57%	11.210%
54	7.551	2015	2025	2048	rBV	195081	365408	13.92%	1.986%
55	7.960	2150	2152	2156	rBV3	615	328	0.01%	0.002%
56	8.024	2164	2172	2204	rBV2	314299	680747	25.94%	3.701%
57	8.535	2329	2331	2332	rBV2	691	215	0.01%	0.001%
58	8.667	2368	2372	2375	rBV4	1156	806	0.03%	0.004%
59	8.780	2396	2407	2433	rBV	1067360	1774437	67.60%	9.646%
60	9.201	2532	2538	2542	rBV5	1071	1184	0.05%	0.006%
61	9.236	2547	2549	2551	rVB2	630	252	0.01%	0.001%
62	9.265	2557	2558	2560	rVB	358	102	0.00%	0.001%
63	9.291	2560	2566	2569	rBV5	644	651	0.02%	0.004%
64	9.307	2569	2571	2575	rVV4	852	626	0.02%	0.003%
65	9.329	2575	2578	2581	rVB3	989	535	0.02%	0.003%
66	9.426	2606	2608	2614	rVB3	383	292	0.01%	0.002%
67	9.471	2619	2622	2627	rVB5	714	604	0.02%	0.003%
68	9.500	2627	2631	2632	rBV2	512	335	0.01%	0.002%
69	9.580	2653	2656	2659	rVB3	292	180	0.01%	0.001%
70	9.612	2659	2666	2669	rVB4	863	901	0.03%	0.005%
71	9.625	2669	2670	2671	rBV4	396	107	0.00%	0.001%
72	9.638	2671	2674	2680	rVB4	450	390	0.01%	0.002%
73	9.686	2686	2689	2693	rBV2	670	474	0.02%	0.003%
74	9.725	2698	2701	2702	rBV2	625	400	0.02%	0.002%
75	9.760	2711	2712	2715	rVB2	572	238	0.01%	0.001%
76	9.783	2715	2719	2722	rBV5	607	492	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037743.D
 Acq On : 04 Oct 2024 15:27
 Operator : SY/MD
 Sample : P4284-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	9.844	2734	2738	2741	rBV3	455	347	0.01%	0.002%
78	9.860	2741	2743	2745	rBV2	385	256	0.01%	0.001%
79	9.931	2761	2765	2767	rBV2	662	395	0.02%	0.002%
80	9.960	2771	2774	2778	rVV4	620	520	0.02%	0.003%
81	10.146	2818	2832	2863	rBV	663492	1065430	40.59%	5.792%
82	10.445	2923	2925	2929	rVB2	990	638	0.02%	0.003%
83	10.529	2949	2951	2953	rBV2	562	257	0.01%	0.001%
84	10.693	3001	3002	3007	rVB	735	510	0.02%	0.003%
85	10.715	3007	3009	3011	rBV	436	194	0.01%	0.001%
86	10.857	3049	3053	3055	rVB3	690	433	0.02%	0.002%
87	10.876	3055	3059	3063	rBV3	487	441	0.02%	0.002%
88	10.976	3088	3090	3092	rBV	169	95	0.00%	0.001%
89	10.989	3092	3094	3097	rBV2	384	251	0.01%	0.001%
90	11.069	3115	3119	3122	rBV3	691	732	0.03%	0.004%
91	11.114	3131	3133	3135	rBV3	584	390	0.01%	0.002%
92	11.127	3135	3137	3141	rVB3	1190	735	0.03%	0.004%
93	11.178	3142	3153	3186	rBV	1036815	1663589	63.38%	9.043%
94	11.554	3257	3270	3297	rBV	1177480	1863663	71.00%	10.131%
95	11.950	3390	3393	3394	rBV2	558	264	0.01%	0.001%
96	12.152	3453	3456	3458	rBV2	746	427	0.02%	0.002%
97	12.339	3511	3514	3517	rBV3	998	674	0.03%	0.004%
98	12.731	3634	3636	3640	rBV4	660	534	0.02%	0.003%
99	12.802	3653	3658	3660	rBV4	906	848	0.03%	0.005%
100	13.185	3775	3777	3781	rBV2	636	278	0.01%	0.002%




Sum of corrected areas: 18395482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037743.D
Acq On : 04 Oct 2024 15:27
Operator : SY/MD
Sample : P4284-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

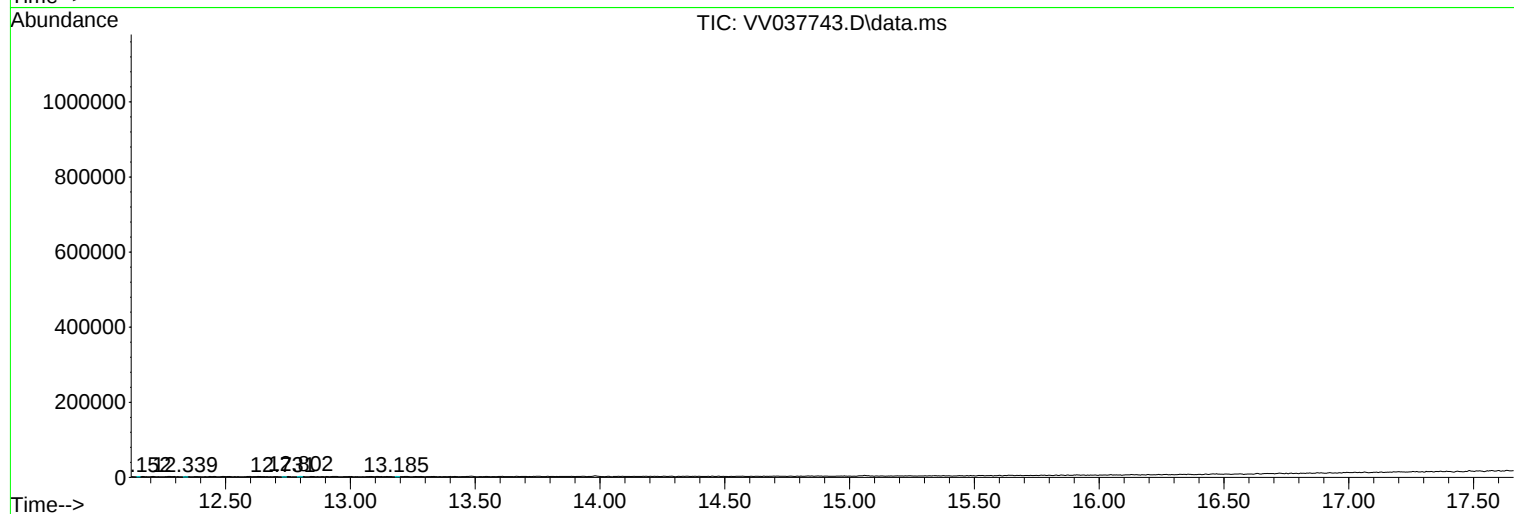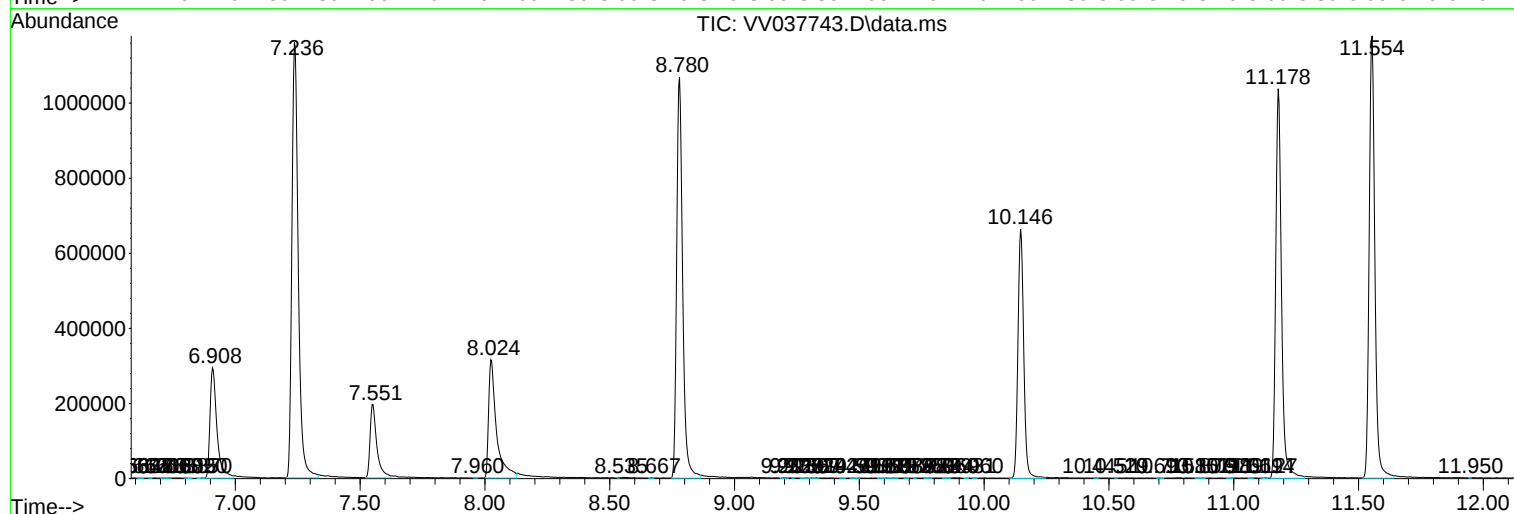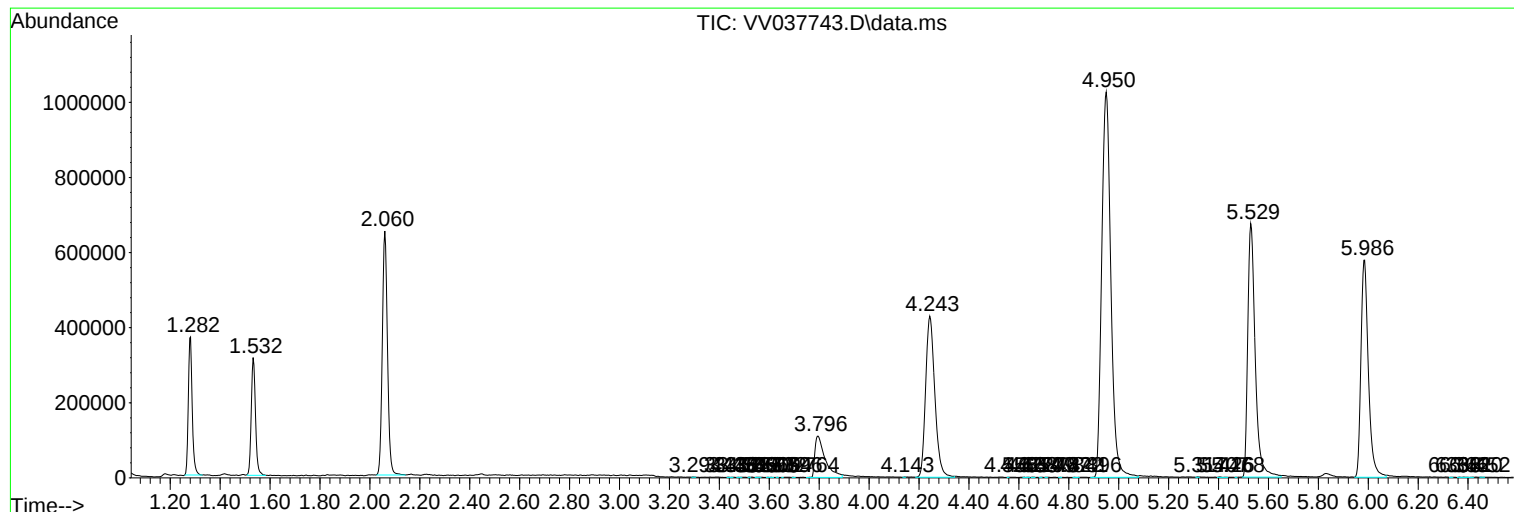

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037743.D
Acq On : 04 Oct 2024 15:27
Operator : SY/MD
Sample : P4284-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037743.D
Acq On : 04 Oct 2024 15:27
Operator : SY/MD
Sample : P4284-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc