

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037744.D
 Acq On : 04 Oct 2024 15:49
 Operator : SY/MD
 Sample : VIBLK399
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK399

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	38	44	50	rBV2	4574	7884	0.30%	0.042%
2	1.278	67	74	92	rVB	359311	391165	14.91%	2.096%
3	1.532	145	153	172	rVB	310813	369623	14.09%	1.980%
4	2.059	307	317	339	rVB	639900	923320	35.19%	4.947%
5	3.252	686	688	692	rBV3	858	605	0.02%	0.003%
6	3.313	705	707	711	rVB5	803	564	0.02%	0.003%
7	3.336	711	714	718	rVB3	797	700	0.03%	0.004%
8	3.365	718	723	728	rBV5	857	784	0.03%	0.004%
9	3.628	802	805	806	rBV2	764	417	0.02%	0.002%
10	3.702	824	828	831	rBV5	685	479	0.02%	0.003%
11	3.796	848	857	890	rBV	116621	354581	13.52%	1.900%
12	4.243	978	996	1028	rBV	422979	1088225	41.48%	5.830%
13	4.471	1065	1067	1072	rVB5	796	644	0.02%	0.003%
14	4.500	1074	1076	1081	rVB3	1185	1022	0.04%	0.005%
15	4.558	1092	1094	1099	rVB6	614	463	0.02%	0.002%
16	4.625	1112	1115	1121	rVB3	1157	919	0.04%	0.005%
17	4.664	1121	1127	1130	rBV4	1133	994	0.04%	0.005%
18	4.699	1135	1138	1143	rVB4	765	669	0.03%	0.004%
19	4.767	1156	1159	1162	rVB2	671	417	0.02%	0.002%
20	4.882	1192	1195	1199	rBV3	903	766	0.03%	0.004%
21	4.950	1199	1216	1244	rBV2	1041717	2623483	100.00%	14.056%
22	5.210	1295	1297	1301	rBV4	1161	999	0.04%	0.005%
23	5.230	1301	1303	1308	rVB5	1314	783	0.03%	0.004%
24	5.252	1308	1310	1312	rBV3	797	403	0.02%	0.002%
25	5.410	1357	1359	1363	rBV4	782	509	0.02%	0.003%
26	5.529	1383	1396	1433	rBV	683768	1431365	54.56%	7.669%
27	5.831	1481	1490	1506	rBV4	10665	22295	0.85%	0.119%
28	5.985	1525	1538	1570	rBV	579258	1207365	46.02%	6.469%
29	6.316	1637	1641	1644	rBV2	950	957	0.04%	0.005%
30	6.345	1648	1650	1655	rVB4	953	880	0.03%	0.005%
31	6.423	1667	1674	1675	rBV5	765	810	0.03%	0.004%
32	6.435	1675	1678	1683	rVB4	1096	833	0.03%	0.004%
33	6.461	1683	1686	1688	rBV2	889	517	0.02%	0.003%
34	6.477	1688	1691	1695	rVB5	649	407	0.02%	0.002%
35	6.525	1701	1706	1711	rBV5	730	901	0.03%	0.005%
36	6.696	1753	1759	1760	rBV4	534	480	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037744.D
 Acq On : 04 Oct 2024 15:49
 Operator : SY/MD
 Sample : VIBLK399
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK399

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.783	1784	1786	1788	rBV3	800	446	0.02%	0.002%
38	6.857	1804	1809	1813	rBV3	530	539	0.02%	0.003%
39	6.908	1813	1825	1860	rBV	292316	572129	21.81%	3.065%
40	7.239	1914	1928	1957	rBV	1164586	2068923	78.86%	11.085%
41	7.551	2016	2025	2050	rBV	197007	369392	14.08%	1.979%
42	7.937	2142	2145	2146	rBV2	838	562	0.02%	0.003%
43	7.950	2146	2149	2152	rVV3	1257	887	0.03%	0.005%
44	8.024	2163	2172	2220	rBV2	331942	743438	28.34%	3.983%
45	8.548	2331	2335	2336	rBV2	936	763	0.03%	0.004%
46	8.622	2355	2358	2361	rBV4	805	604	0.02%	0.003%
47	8.638	2361	2363	2370	rVB5	760	738	0.03%	0.004%
48	8.779	2396	2407	2442	rBV	1081955	1802130	68.69%	9.655%
49	9.075	2497	2499	2503	rVB5	964	512	0.02%	0.003%
50	9.114	2508	2511	2512	rBV2	752	445	0.02%	0.002%
51	9.287	2563	2565	2567	rVV2	780	436	0.02%	0.002%
52	9.300	2567	2569	2574	rVV4	942	624	0.02%	0.003%
53	9.477	2620	2624	2628	rVB3	566	475	0.02%	0.003%
54	9.609	2661	2665	2666	rVV2	845	502	0.02%	0.003%
55	9.619	2666	2668	2673	rVV4	660	516	0.02%	0.003%
56	9.654	2675	2679	2685	rVB4	770	644	0.02%	0.003%
57	9.683	2685	2688	2691	rBV3	688	453	0.02%	0.002%
58	9.728	2700	2702	2706	rVB2	737	520	0.02%	0.003%
59	9.767	2711	2714	2718	rVB4	809	425	0.02%	0.002%
60	9.840	2732	2737	2739	rBV2	748	547	0.02%	0.003%
61	9.998	2779	2786	2789	rBV5	868	1046	0.04%	0.006%
62	10.049	2798	2802	2804	rBV2	771	422	0.02%	0.002%
63	10.069	2804	2808	2810	rBV2	668	514	0.02%	0.003%
64	10.146	2820	2832	2858	rBV	683896	1091291	41.60%	5.847%
65	10.628	2980	2982	2986	rVB4	752	486	0.02%	0.003%
66	10.651	2986	2989	2991	rBV	678	427	0.02%	0.002%
67	10.718	3006	3010	3013	rBV2	767	651	0.02%	0.003%
68	10.766	3020	3025	3028	rBV3	667	650	0.02%	0.003%
69	10.786	3028	3031	3035	rVV3	1353	1332	0.05%	0.007%
70	10.889	3058	3063	3066	rBV2	691	571	0.02%	0.003%
71	11.014	3099	3102	3105	rBV3	658	477	0.02%	0.003%
72	11.136	3135	3140	3142	rBV3	989	848	0.03%	0.005%
73	11.178	3142	3153	3192	rVV	1052357	1684630	64.21%	9.026%
74	11.554	3258	3270	3298	rBV	1158872	1860588	70.92%	9.968%
75	11.779	3337	3340	3343	rBV3	780	554	0.02%	0.003%
76	11.818	3350	3352	3355	rVB4	1095	496	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
 Data File : VV037744.D
 Acq On : 04 Oct 2024 15:49
 Operator : SY/MD
 Sample : VIBLK399
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK399

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.882	3369	3372	3376	rVB3	1100	901	0.03%	0.005%
78	11.905	3376	3379	3380	rBV	898	479	0.02%	0.003%
79	12.027	3414	3417	3420	rVB3	723	477	0.02%	0.003%
80	12.078	3428	3433	3436	rBV4	831	896	0.03%	0.005%
81	12.181	3461	3465	3468	rBV4	811	737	0.03%	0.004%
82	12.297	3499	3501	3506	rBV4	518	420	0.02%	0.002%
83	12.393	3525	3531	3532	rBV2	568	482	0.02%	0.003%
84	12.503	3562	3565	3569	rBV4	810	604	0.02%	0.003%
85	12.580	3584	3589	3594	rBV3	695	690	0.03%	0.004%
86	12.606	3594	3597	3602	rVB4	864	729	0.03%	0.004%
87	12.699	3623	3626	3628	rBV3	658	420	0.02%	0.002%
88	12.741	3635	3639	3640	rBV2	774	546	0.02%	0.003%
89	12.985	3712	3715	3717	rBV4	902	551	0.02%	0.003%
90	13.191	3776	3779	3783	rVB4	899	636	0.02%	0.003%
91	13.223	3783	3789	3790	rBV4	815	873	0.03%	0.005%
92	13.326	3818	3821	3824	rBV4	754	447	0.02%	0.002%
93	13.445	3854	3858	3859	rBV3	828	584	0.02%	0.003%
94	13.564	3892	3895	3900	rBV2	707	682	0.03%	0.004%
95	13.638	3914	3918	3921	rBV4	953	821	0.03%	0.004%
96	13.786	3958	3964	3966	rBV3	941	1100	0.04%	0.006%
97	14.168	4080	4083	4084	rBV2	724	427	0.02%	0.002%
98	14.258	4109	4111	4116	rBV6	615	572	0.02%	0.003%
99	14.438	4164	4167	4172	rBV5	956	1048	0.04%	0.006%
100	14.673	4237	4240	4243	rBV4	1209	892	0.03%	0.005%




Sum of corrected areas: 18664875

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037744.D
Acq On : 04 Oct 2024 15:49
Operator : SY/MD
Sample : VIBLK399
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK399

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

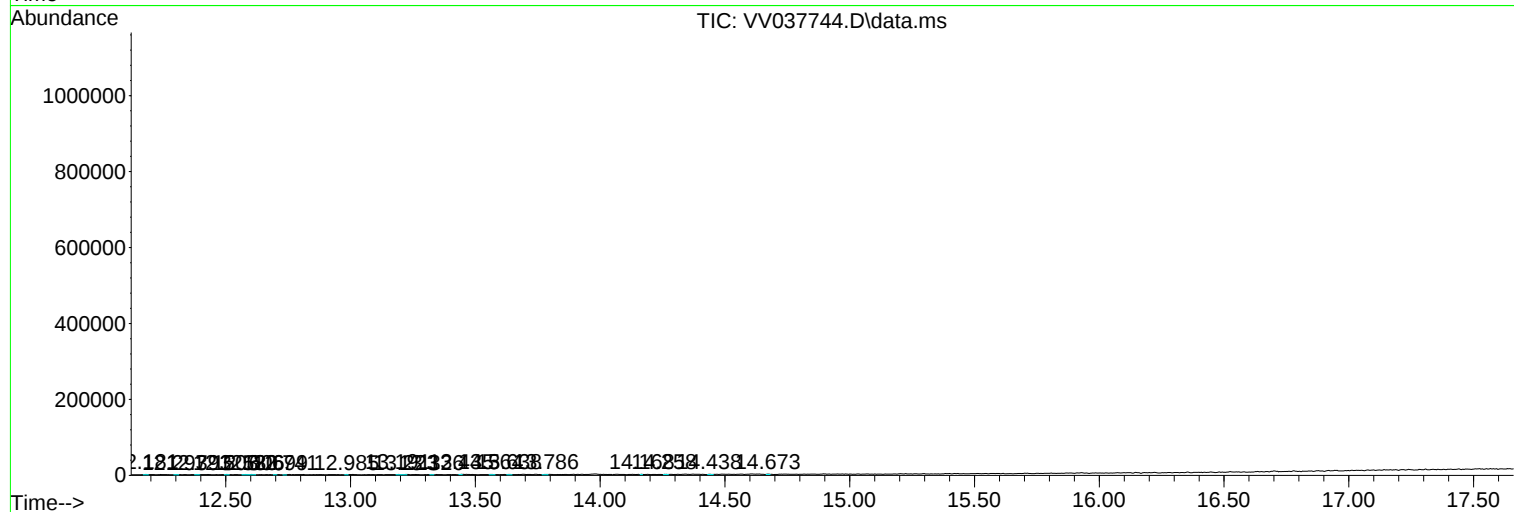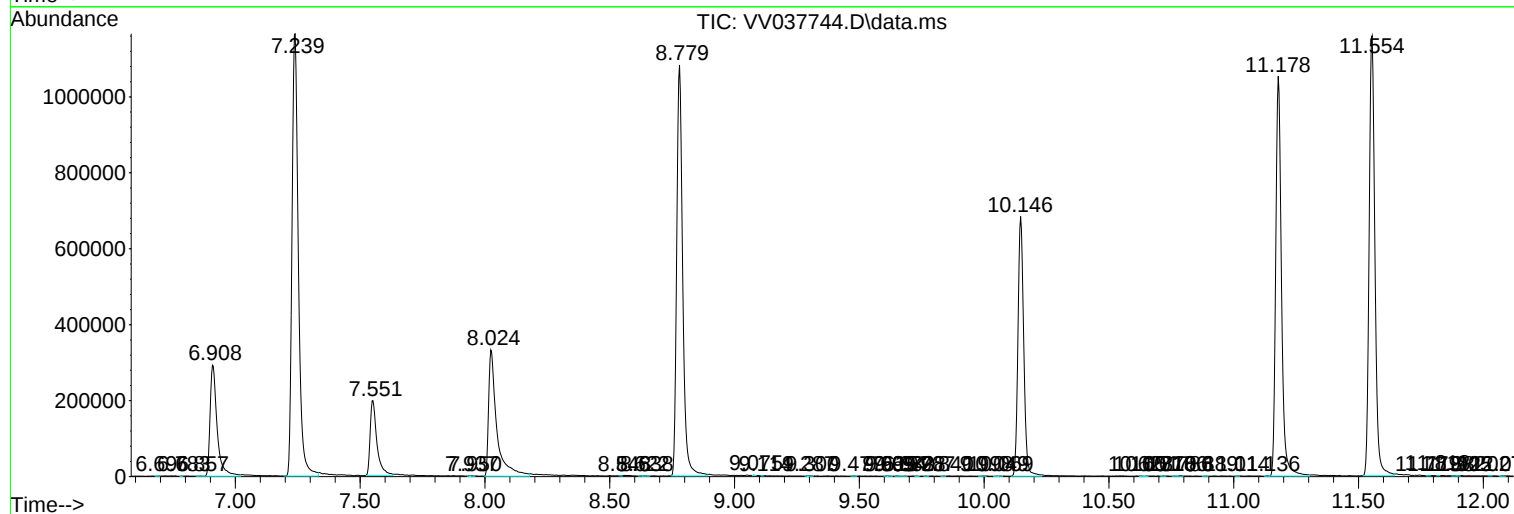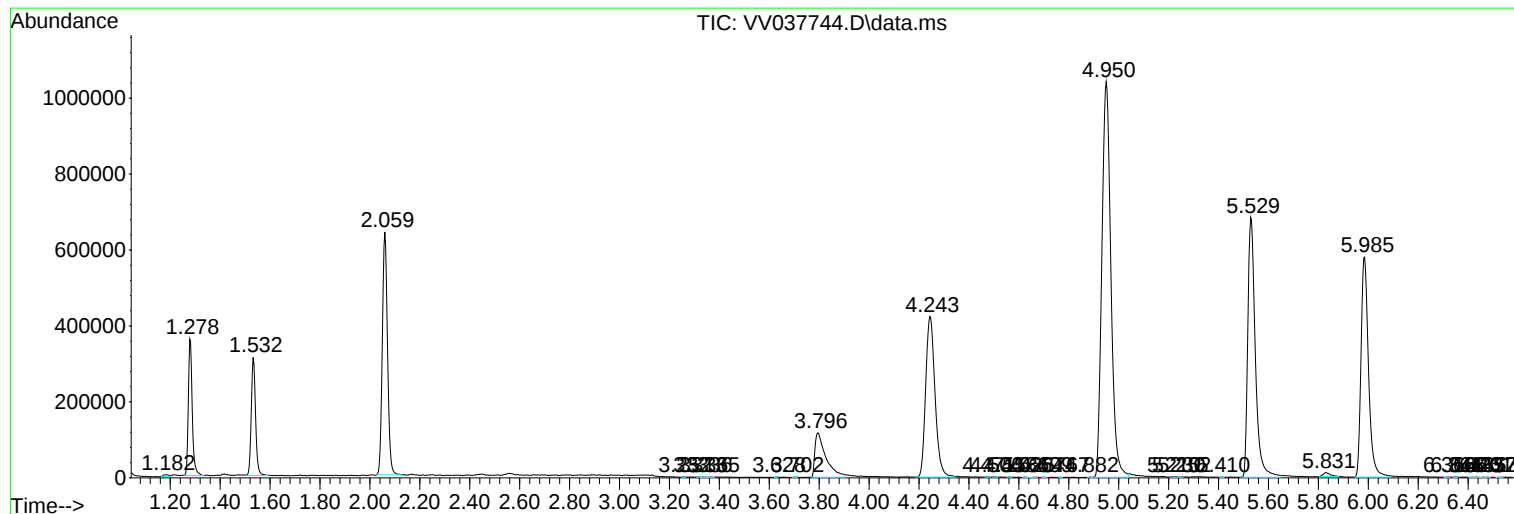

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037744.D
Acq On : 04 Oct 2024 15:49
Operator : SY/MD
Sample : VIBLK399
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK399

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037744.D
Acq On : 04 Oct 2024 15:49
Operator : SY/MD
Sample : VIBLK399
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK399

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------