
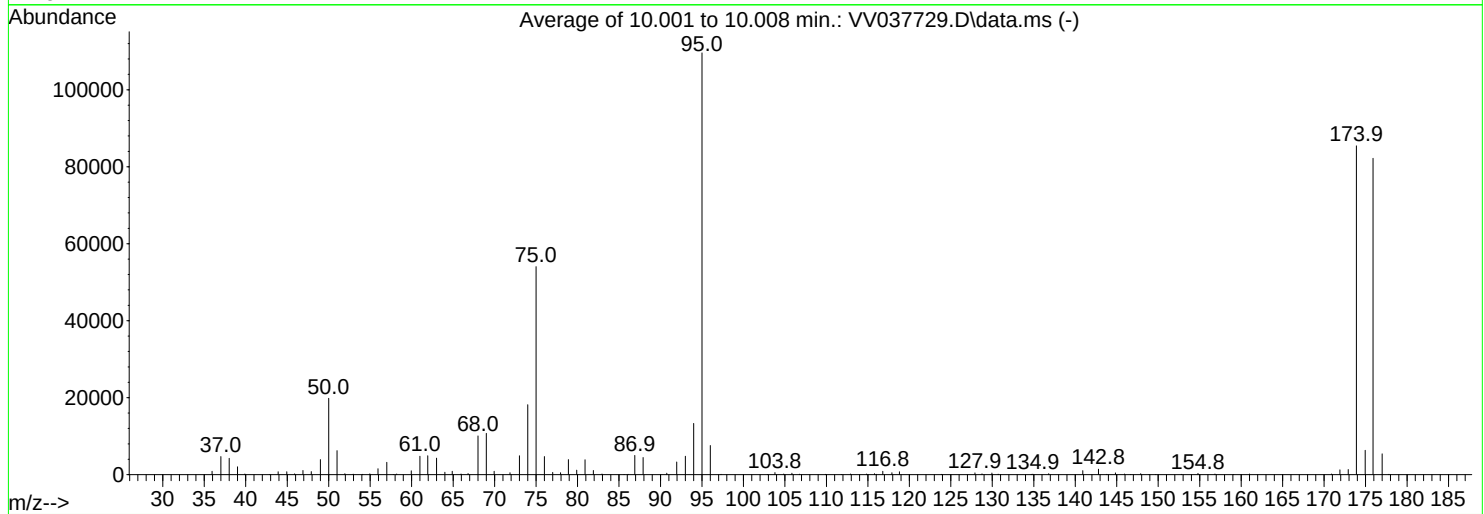


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100424\
Data File : VV037729.D
Acq On : 04 Oct 2024 07:52
Operator : SY/MD
Sample : BFB387
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB387

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Mon Oct 07 04:10:13 2024

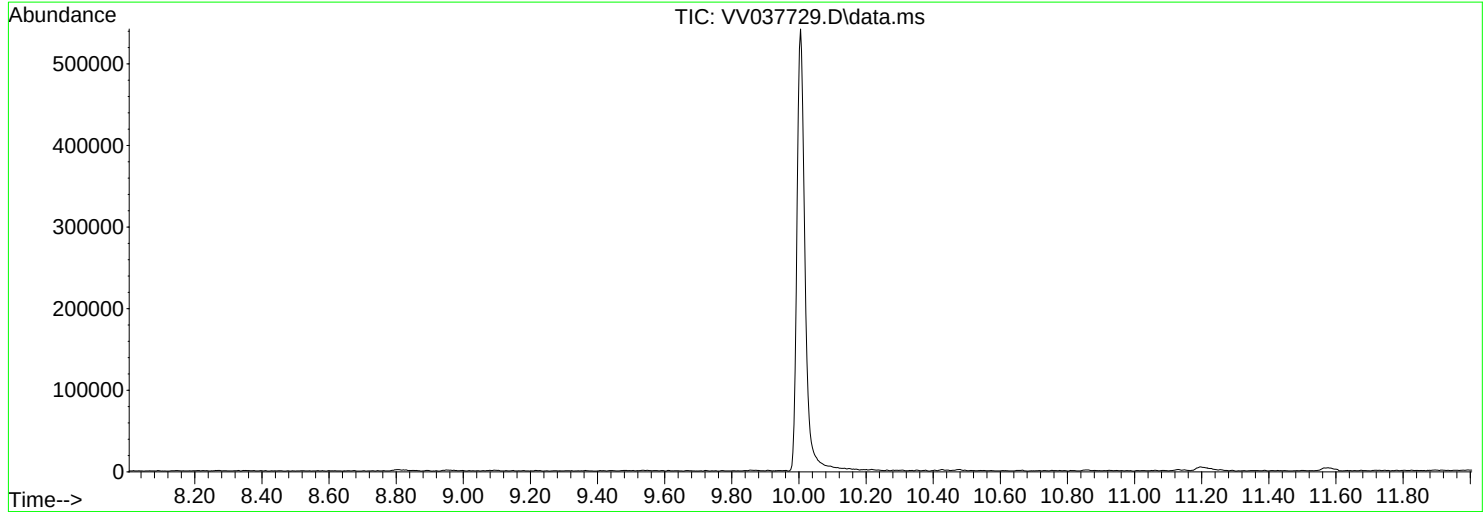

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	19813	PASS
75	95	30	80	49.3	54035	PASS
95	95	100	100	100.0	109597	PASS
96	95	5	9	6.9	7582	PASS
173	174	0.00	2	1.6	1336	PASS
174	95	50	120	77.9	85424	PASS
175	174	5	9	7.4	6337	PASS
176	174	95	105	96.2	82187	PASS
177	176	5	10	6.6	5392	PASS

m/z	Abundance
39.90	278.0
40.90	126.0
43.90	603.0
76.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
36.00	921.0
37.00	4599.0
38.00	4202.0
39.00	2117.0
39.90	405.0
43.90	1205.0
45.00	771.0
45.90	188.0
46.90	1134.0
47.90	847.0
49.00	4077.0
50.00	19392.0
51.00	6070.0
52.00	214.0
52.90	125.0
54.90	199.0
55.90	1421.0
57.00	3243.0
57.80	110.0
58.20	165.0
59.90	965.0
61.00	4695.0
62.00	4906.0
63.00	4064.0
64.00	585.0
64.90	1030.0
66.00	170.0
66.80	373.0
68.00	10353.0
69.00	11163.0
70.00	852.0
71.80	510.0
73.00	4870.0
74.00	17920.0
75.00	54352.0
76.00	4697.0
77.10	693.0
78.00	518.0
78.90	3870.0
79.90	1109.0
80.90	4031.0
81.90	1104.0
82.90	157.0
86.90	5141.0
87.90	4088.0
90.70	368.0
91.90	3198.0
93.00	4644.0
94.00	13257.0
95.00	109824.0
96.00	7442.0
102.90	147.0
103.80	589.0
104.80	187.0
105.80	439.0
106.70	133.0
111.80	118.0
112.90	146.0
114.80	174.0
115.80	365.0
116.80	873.0
117.90	514.0
118.80	696.0
123.90	178.0
127.90	452.0
128.80	255.0
130.00	401.0
131.00	123.0
134.70	255.0
136.80	217.0
140.90	1116.0
142.80	1400.0
144.90	497.0
145.90	180.0
147.90	241.0
154.80	309.0
156.90	127.0
161.00	126.0
171.00	164.0
171.90	1187.0
172.90	1260.0
173.90	82384.0
175.00	6408.0
175.90	79328.0
177.00	5128.0
177.80	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
36.00	885.0
37.00	4833.0
38.00	4390.0
39.00	2075.0
39.90	473.0
43.90	1394.0
44.90	767.0
45.90	204.0
46.90	1070.0
47.90	814.0
49.00	4049.0
50.00	20464.0
51.00	6495.0
52.00	259.0
52.90	110.0
54.10	124.0
54.90	196.0
55.90	1609.0
57.00	3342.0
58.20	171.0
60.00	996.0
61.00	4908.0
61.90	5070.0
63.00	4382.0
64.00	661.0
64.90	878.0
66.00	182.0
66.80	318.0
68.00	10249.0
69.00	11048.0
69.90	909.0
71.90	529.0
73.00	5054.0
74.00	18800.0
75.00	55736.0
76.00	4802.0
77.10	735.0
78.00	494.0
78.90	4034.0
79.90	1192.0
80.90	3985.0
81.90	1116.0
82.90	176.0
86.10	141.0
86.90	5123.0
87.90	4669.0
90.80	402.0
91.90	3425.0
93.00	4943.0
94.00	13780.0
95.00	113552.0
96.00	7904.0
97.30	116.0
103.80	563.0
104.90	167.0
105.80	409.0
106.70	142.0
109.90	113.0
112.90	162.0
114.80	181.0
115.80	335.0
116.80	898.0
117.90	528.0
118.80	754.0
123.90	129.0
127.90	483.0
128.70	207.0
130.00	410.0
130.70	174.0
134.90	218.0
136.80	253.0
140.90	1052.0
142.80	1501.0
143.80	114.0
144.90	500.0
146.00	176.0
147.90	266.0
148.90	110.0
152.80	146.0
154.80	335.0
156.90	164.0
161.00	197.0
170.80	155.0
171.90	1249.0
172.90	1400.0
173.90	88408.0
175.00	6473.0
175.90	84672.0
177.00	5601.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
35.90	811.0
37.00	4707.0
38.00	4139.0
39.00	1882.0
39.90	483.0
42.90	122.0
43.90	1454.0
45.00	776.0
45.90	193.0
46.90	1057.0
47.90	763.0
49.00	3632.0
50.00	19584.0
51.00	6100.0
51.90	285.0
53.00	110.0
54.10	117.0
55.00	209.0
56.00	1638.0
57.00	3011.0
58.20	134.0
60.00	1030.0
61.00	4791.0
61.90	4742.0
63.00	4360.0
64.00	648.0
64.90	749.0
65.90	171.0
66.90	223.0
68.00	9576.0
69.00	9997.0
69.90	869.0
71.90	529.0
73.00	4834.0
74.00	17824.0
75.00	52016.0
76.00	4545.0
76.90	711.0
77.90	504.0
78.90	3780.0
79.90	1165.0
80.90	3603.0
81.90	1065.0
83.00	174.0
85.60	136.0
86.10	179.0
86.90	4667.0
87.90	4587.0
90.80	422.0
92.00	3198.0
93.00	4755.0
94.00	12885.0
95.00	105416.0
96.00	7400.0
97.30	156.0
103.80	525.0
104.90	131.0
105.90	308.0
106.80	120.0
109.90	107.0
112.90	174.0
114.90	158.0
116.00	322.0
116.80	860.0
117.90	474.0
118.80	764.0
127.90	503.0
128.80	130.0
129.80	435.0
130.70	202.0
134.90	173.0
136.80	260.0
140.90	940.0
142.80	1367.0
143.80	104.0
144.80	434.0
146.00	169.0
146.70	107.0
147.90	238.0
149.70	103.0
152.80	147.0
154.80	357.0
156.80	162.0
159.10	112.0
161.00	188.0
170.90	166.0
171.90	1249.0
172.90	1348.0
173.90	85480.0
174.90	6131.0
175.90	82560.0
177.00	5448.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

177.80

135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387