

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028360.D
 Acq On : 05 Oct 2022 11:51
 Operator : SY/MD
 Sample : VV1005WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Quant Time: Oct 06 02:31:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	183497	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	179661	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	85574	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	59821	4.339	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.800%	
7) Chloroethane-d5	1.561	69	57640	4.938	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.800%	
11) 1,1-Dichloroethene-d2	2.102	63	88861	3.419	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	3.925	46	116097	49.767	ug/L	0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.540%	
24) Chloroform-d	4.339	84	127546	5.106	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
26) 1,2-Dichloroethane-d4	5.027	65	60833	5.253	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.000%	
32) Benzene-d6	5.040	84	266769	5.413	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	108.200%	
36) 1,2-Dichloropropane-d6	6.063	67	81732	5.781	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.600%	
41) Toluene-d8	7.310	98	218679	4.825	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.619	79	25922	4.814	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.200%	
46) 2-Hexanone-d5	8.088	63	108915	49.417	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.840%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	54076	5.046	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	11.619	152	82231	5.584	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	4229	0.285	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028360.D
Acq On : 05 Oct 2022 11:51
Operator : SY/MD
Sample : VV1005WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248


Quant Time: Oct 06 02:31:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

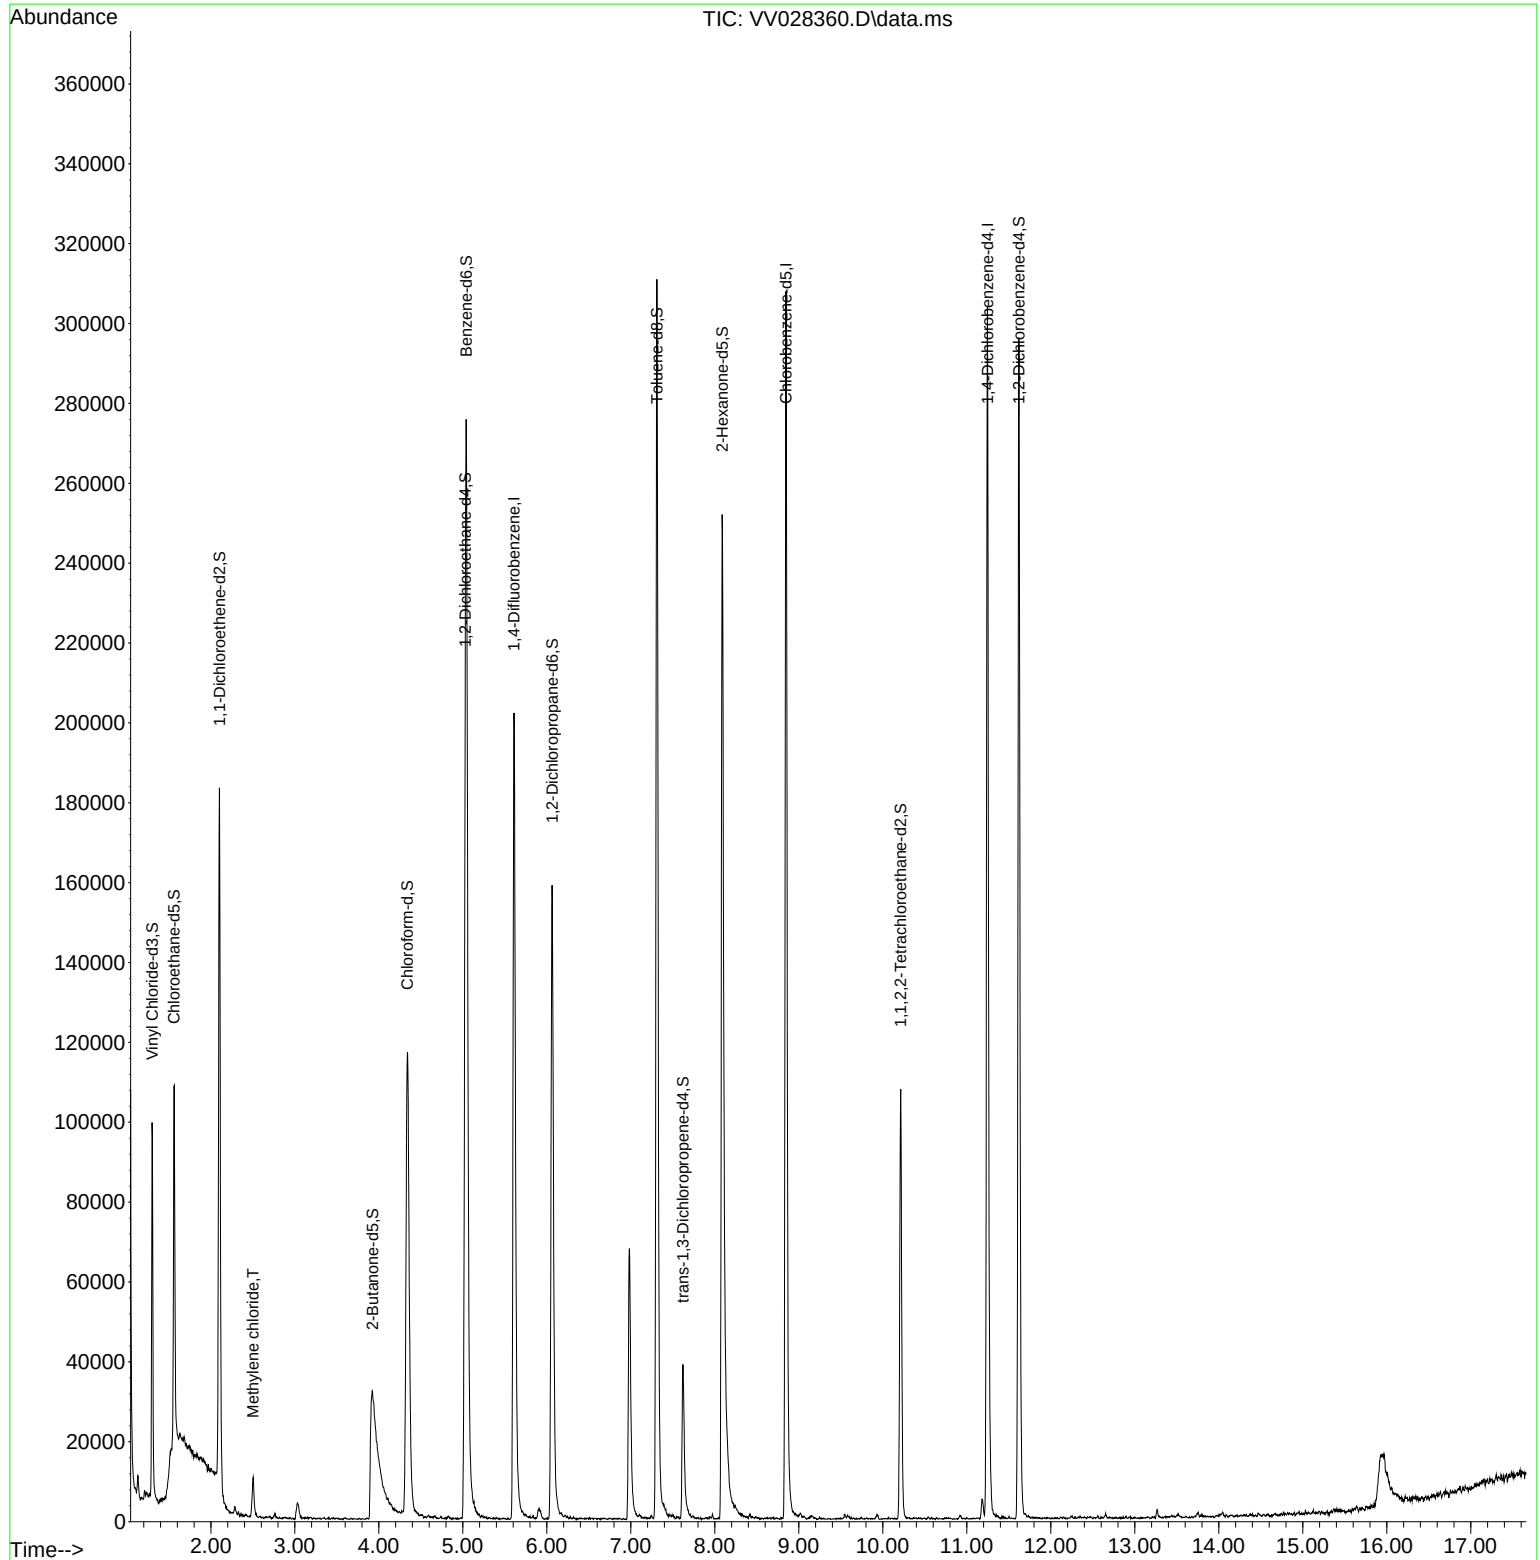

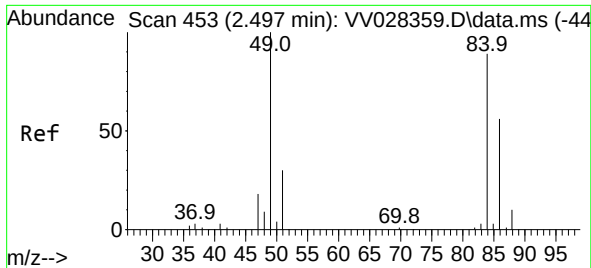

#16
Methylene chloride
Concen: 0.285 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028360.D
Acq: 05 Oct 2022 11:51

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

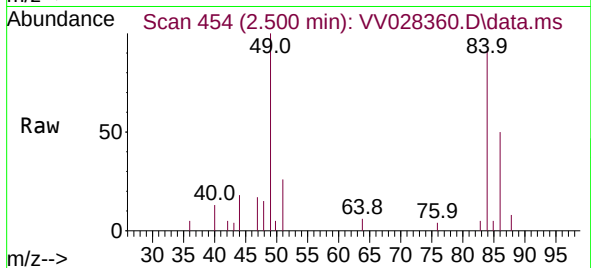

Tgt Ion:	84	Resp:	4229
Ion	Ratio	Lower	Upper
84	100		
86	55.2	46.8	86.8
49	115.0	87.5	162.5

