

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100522\
 Data File : VW028366.D
 Acq On : 05 Oct 2022 14:19
 Operator : SY/MD
 Sample : N4899-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H13

Quant Time: Oct 06 02:32:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 04 02:28:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	192890	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	193023	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	91271	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	53041	3.660	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.564	69	53086	4.327	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.600%
11) 1,1-Dichloroethene-d2	2.105	63	81318	2.977	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.600%#
20) 2-Butanone-d5	3.915	46	153040	62.408	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.820%
24) Chloroform-d	4.342	84	130335	4.964	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
26) 1,2-Dichloroethane-d4	5.031	65	61854	5.081	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.043	84	247569	4.676	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.066	67	78587	5.174	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.313	98	198416	4.074	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	7.622	79	25880	4.473	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%
46) 2-Hexanone-d5	8.088	63	126665	53.493	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.980%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	61676	5.357	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	77809	4.954	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.979	164	608	0.048	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028366.D
Acq On : 05 Oct 2022 14:19
Operator : SY/MD
Sample : N4899-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H13


Quant Time: Oct 06 02:32:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 04 02:28:45 2022
Response via : Initial Calibration

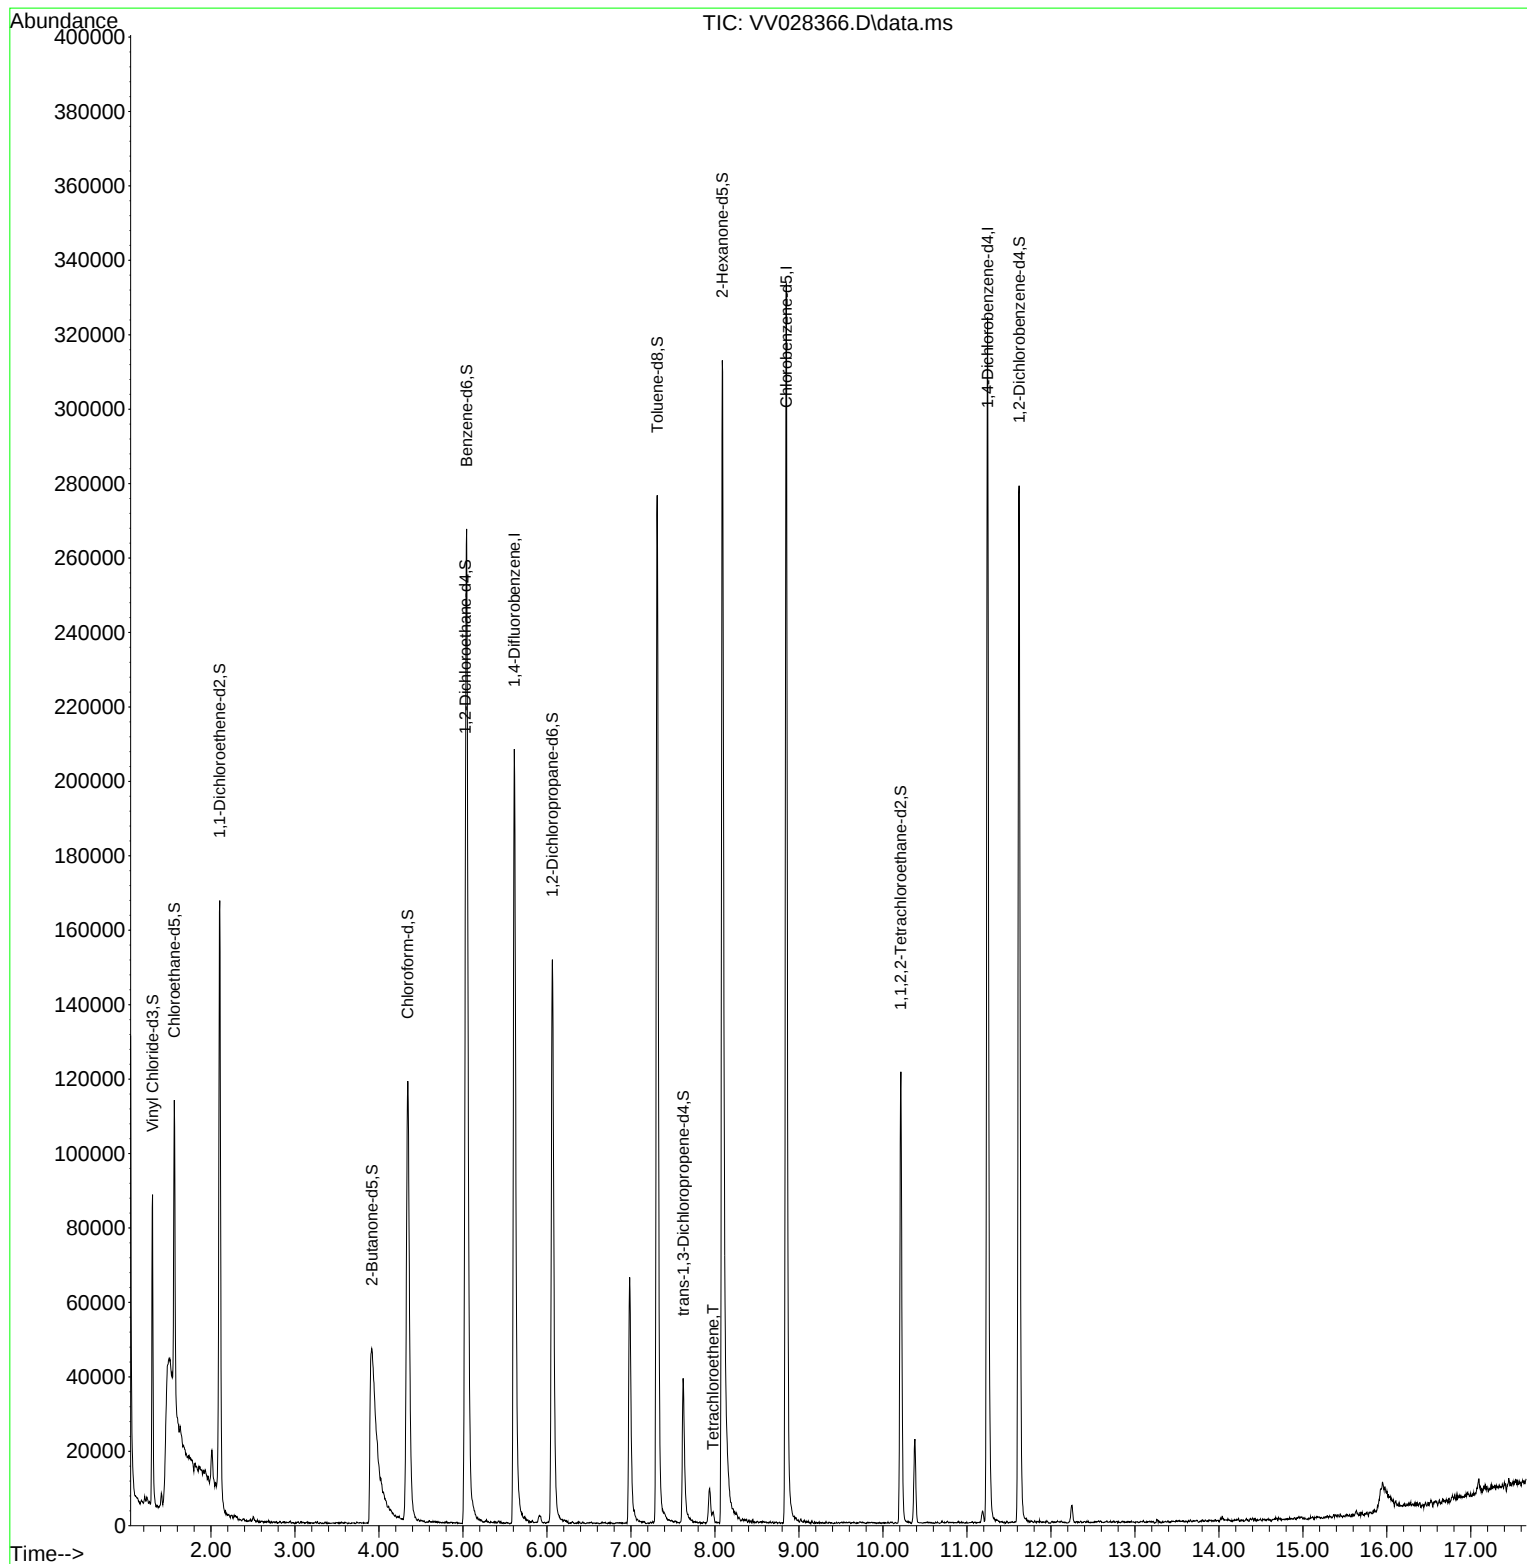

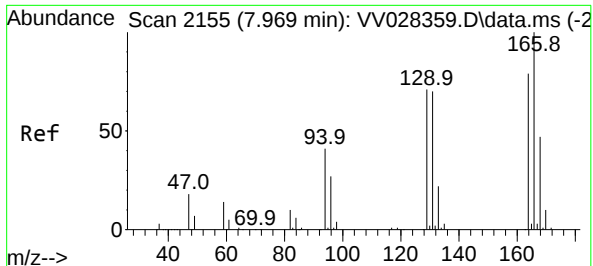

#47
Tetrachloroethene
Concen: 0.048 ug/L
RT: 7.979 min Scan# 21
Delta R.T. 0.010 min
Lab File: VV028366.D
Acq: 05 Oct 2022 14:19

Instrument :
MSVOA_V
ClientSampleId :
F5H13

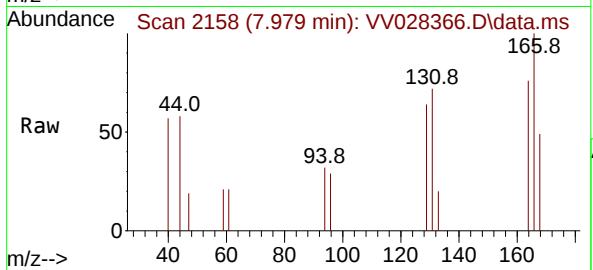

Tgt Ion:	164	Resp:	608
Ion	Ratio	Lower	Upper
164	100		
129	83.6	66.7	123.9
131	94.0	61.7	114.5
166	131.3	90.9	168.9

