

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028360.D
 Acq On : 05 Oct 2022 11:51
 Operator : SY/MD
 Sample : VV1005WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.131	24	28	38	rVB2	6155	7542	1.10%	0.138%
2	1.301	75	81	100	rVB	94629	97970	14.23%	1.788%
3	1.516	132	148	149	rBV	11644	19221	2.79%	0.351%
4	1.565	156	163	179	rVB	88566	105128	15.27%	1.919%
5	2.102	321	330	343	rVB	177316	263193	38.24%	4.804%
6	2.503	445	455	466	rBV2	9816	15681	2.28%	0.286%
7	3.031	610	619	630	rBV6	4075	9143	1.33%	0.167%
8	3.921	882	896	937	rBV2	32100	189482	27.53%	3.459%
9	4.339	1011	1026	1052	rBV	115170	307642	44.70%	5.615%
10	5.040	1228	1244	1271	rBV2	275233	688298	100.00%	12.563%
11	5.609	1404	1421	1450	rBV	201959	414445	60.21%	7.565%
12	6.063	1549	1562	1591	rBV	158709	334272	48.57%	6.101%
13	6.982	1838	1848	1873	rBV2	67868	134907	19.60%	2.462%
14	7.310	1936	1950	1974	rBV	310362	552728	80.30%	10.089%
15	7.619	2037	2046	2072	rBV	38410	75306	10.94%	1.375%
16	8.088	2182	2192	2230	rBV	251504	556553	80.86%	10.159%
17	8.847	2417	2428	2454	rBV	307348	513728	74.64%	9.377%
18	10.214	2840	2853	2872	rBV	107572	172807	25.11%	3.154%
19	11.182	3145	3154	3163	rBV6	4974	8764	1.27%	0.160%
20	11.246	3163	3174	3192	rVV	302685	492304	71.52%	8.986%
21	11.619	3277	3290	3311	rBV	295772	486271	70.65%	8.876%
22	15.927	4609	4630	4633	rBV	12918	33266	4.83%	0.607%




Sum of corrected areas: 5478651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028360.D
Acq On : 05 Oct 2022 11:51
Operator : SY/MD
Sample : VV1005WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

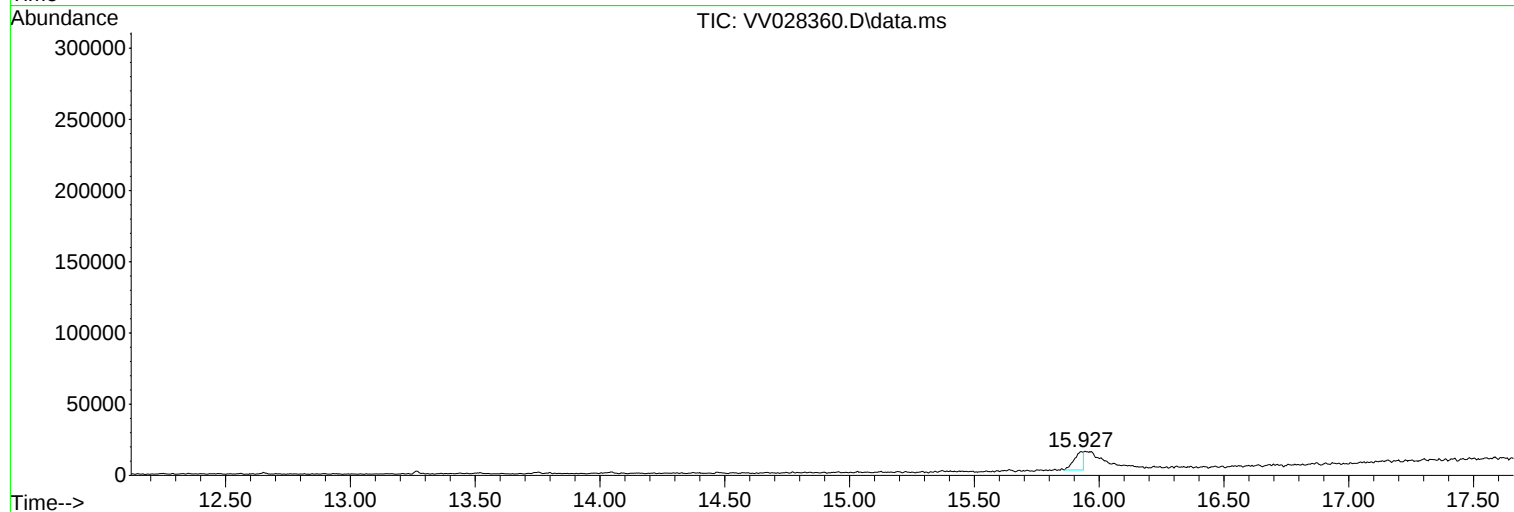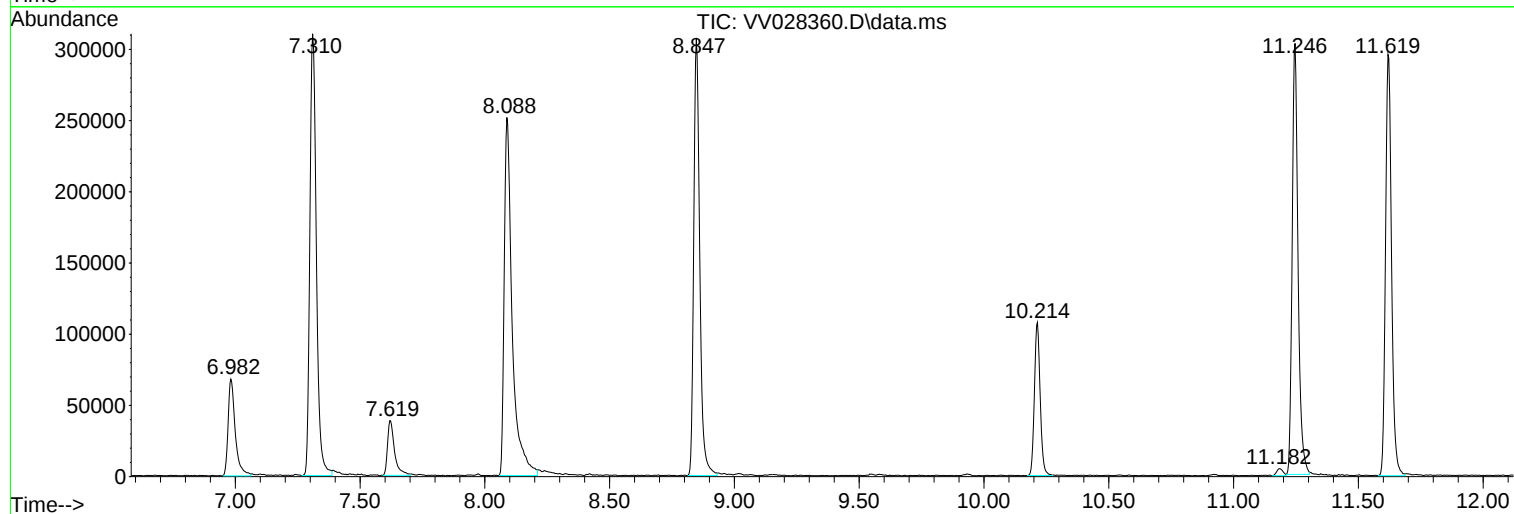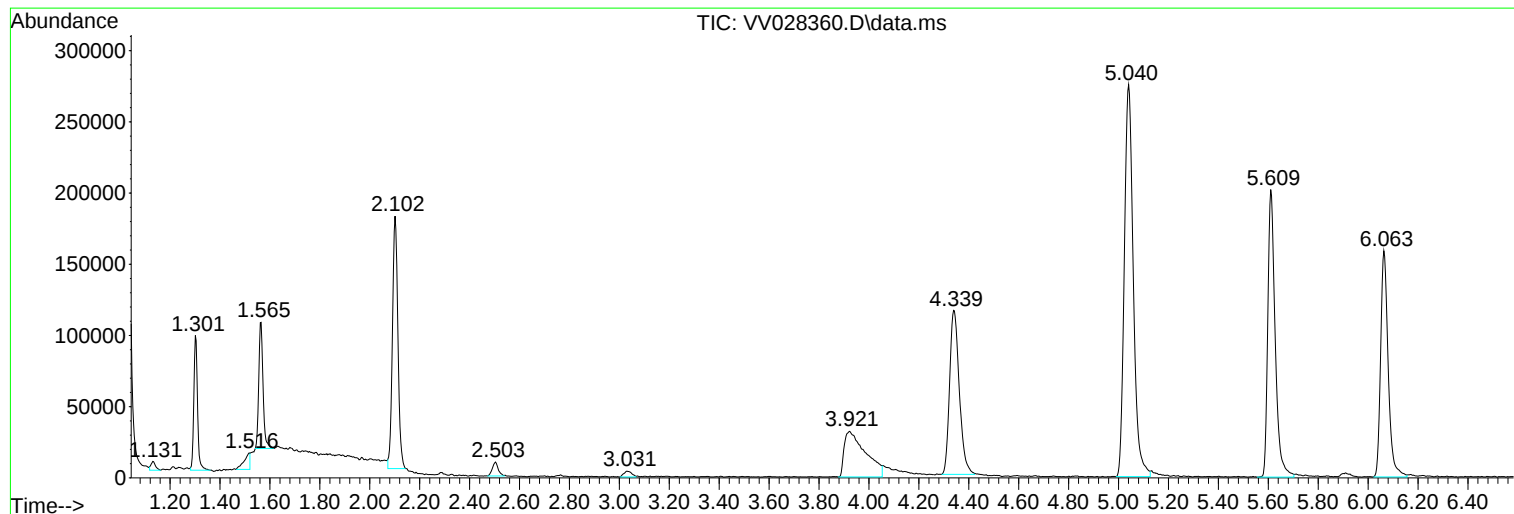

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028360.D
Acq On : 05 Oct 2022 11:51
Operator : SY/MD
Sample : VV1005WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028360.D
Acq On : 05 Oct 2022 11:51
Operator : SY/MD
Sample : VV1005WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc