

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028361.D
 Acq On : 05 Oct 2022 12:21
 Operator : SY/MD
 Sample : N4899-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	86139	88716	14.03%	1.634%
2	1.565	144	163	173	rBV	90404	132582	20.97%	2.442%
3	2.102	321	330	343	rVB	160949	237066	37.49%	4.367%
4	2.500	445	454	467	rVB4	6108	10145	1.60%	0.187%
5	3.037	607	621	633	rBV8	3401	7426	1.17%	0.137%
6	3.918	880	895	935	rBV	35027	195907	30.98%	3.609%
7	4.339	1009	1026	1057	rBV	105246	282624	44.70%	5.206%
8	5.040	1223	1244	1276	rBV2	251707	632333	100.00%	11.649%
9	5.609	1406	1421	1451	rBV2	236896	494326	78.17%	9.106%
10	6.063	1550	1562	1589	rBV2	143346	305456	48.31%	5.627%
11	6.982	1836	1848	1879	rBV	62159	123689	19.56%	2.279%
12	7.310	1938	1950	1976	rBV	275400	494036	78.13%	9.101%
13	7.622	2035	2047	2066	rBV	35246	67869	10.73%	1.250%
14	8.088	2181	2192	2232	rBV	244235	534407	84.51%	9.845%
15	8.847	2417	2428	2456	rBV	368869	608850	96.29%	11.216%
16	10.214	2841	2853	2872	rBV	102499	165502	26.17%	3.049%
17	10.381	2894	2905	2914	rVB2	6595	11201	1.77%	0.206%
18	11.246	3163	3174	3202	rVV	363361	583923	92.34%	10.757%
19	11.619	3277	3290	3310	rBV	268500	441834	69.87%	8.139%
20	15.924	4614	4629	4630	rBV7	6728	10405	1.65%	0.192%




Sum of corrected areas: 5428297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028361.D
Acq On : 05 Oct 2022 12:21
Operator : SY/MD
Sample : N4899-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

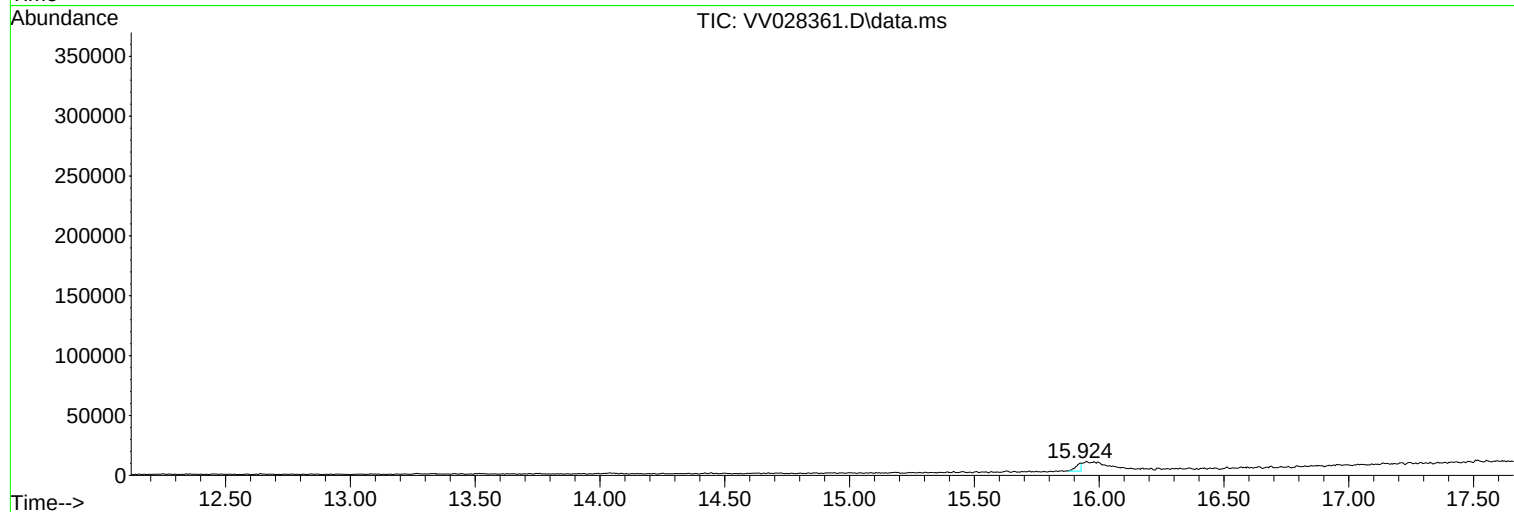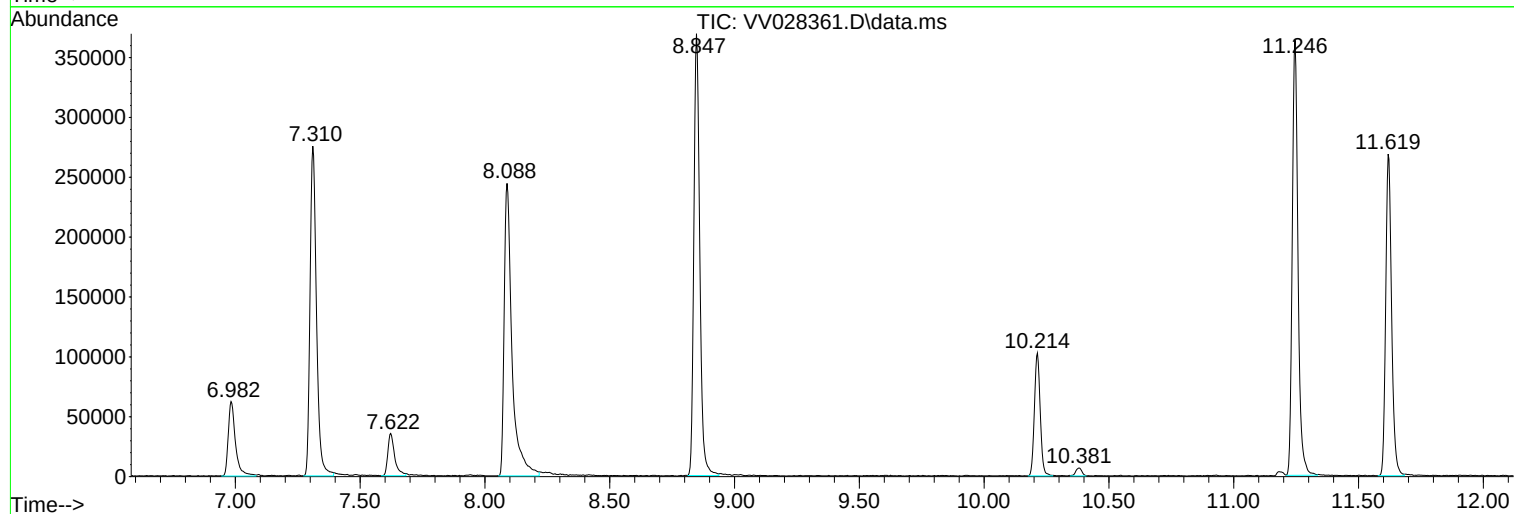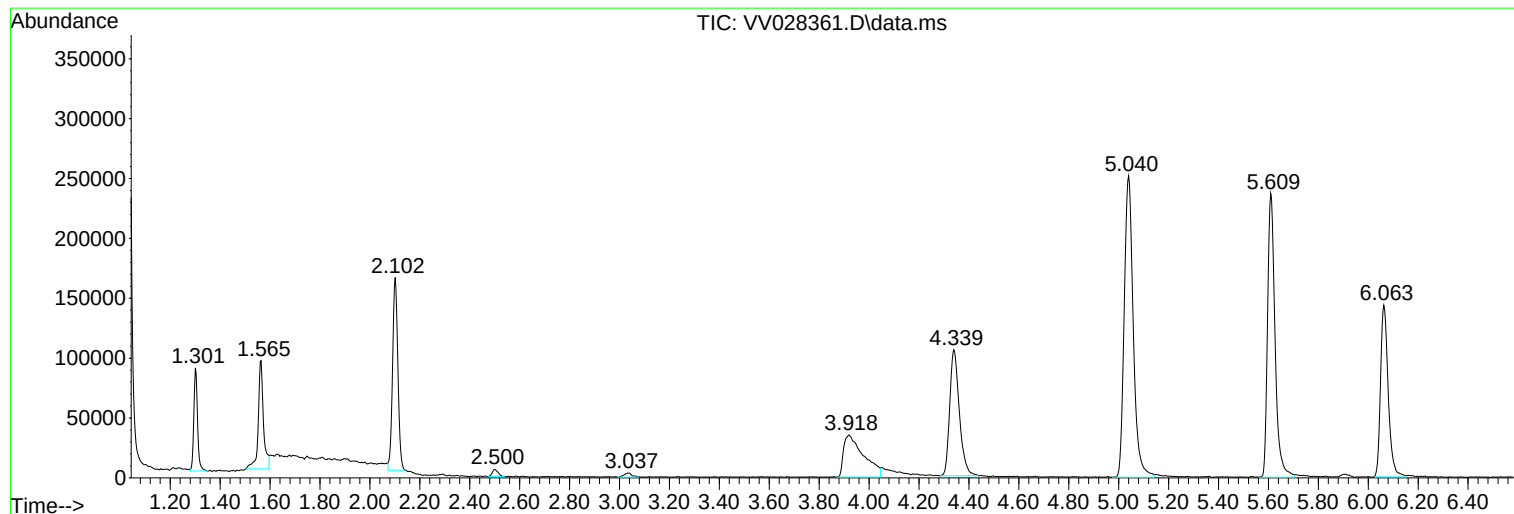

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028361.D
Acq On : 05 Oct 2022 12:21
Operator : SY/MD
Sample : N4899-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028361.D
Acq On : 05 Oct 2022 12:21
Operator : SY/MD
Sample : N4899-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc