

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028362.D
 Acq On : 05 Oct 2022 12:45
 Operator : SY/MD
 Sample : N4899-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	89482	89514	6.22%	1.226%
2	1.516	127	148	149	rBV8	28195	65858	4.58%	0.902%
3	1.564	157	163	186	rVB	98559	128969	8.96%	1.767%
4	2.105	321	331	348	rVB	168972	255229	17.74%	3.497%
5	3.908	880	892	941	rBV	51326	268389	18.65%	3.677%
6	4.342	1011	1027	1058	rBV	117602	318135	22.11%	4.358%
7	5.043	1227	1245	1276	rBV2	268112	676804	47.03%	9.272%
8	5.612	1409	1422	1453	rBV	212265	443867	30.84%	6.081%
9	5.915	1505	1516	1532	rBV3	35067	74754	5.19%	1.024%
10	6.066	1547	1563	1582	rBV	157747	328351	22.82%	4.498%
11	6.985	1836	1849	1874	rBV	68383	133929	9.31%	1.835%
12	7.313	1939	1951	1969	rBV	293868	515998	35.86%	7.069%
13	7.622	2037	2047	2061	rBV2	40613	74485	5.18%	1.020%
14	7.972	2138	2156	2178	rBV	850758	1439113	100.00%	19.715%
15	8.088	2182	2192	2220	rBV	335719	673771	46.82%	9.230%
16	8.850	2418	2429	2449	rBV	328750	552569	38.40%	7.570%
17	10.214	2842	2853	2870	rBV	122791	196459	13.65%	2.691%
18	10.381	2891	2905	2917	rBV2	9519	16564	1.15%	0.227%
19	11.246	3163	3174	3194	rBV	324651	531530	36.93%	7.282%
20	11.532	3252	3263	3279	rBV2	12765	25819	1.79%	0.354%
21	11.622	3279	3291	3309	rVV	294637	489428	34.01%	6.705%




Sum of corrected areas: 7299535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028362.D
Acq On : 05 Oct 2022 12:45
Operator : SY/MD
Sample : N4899-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

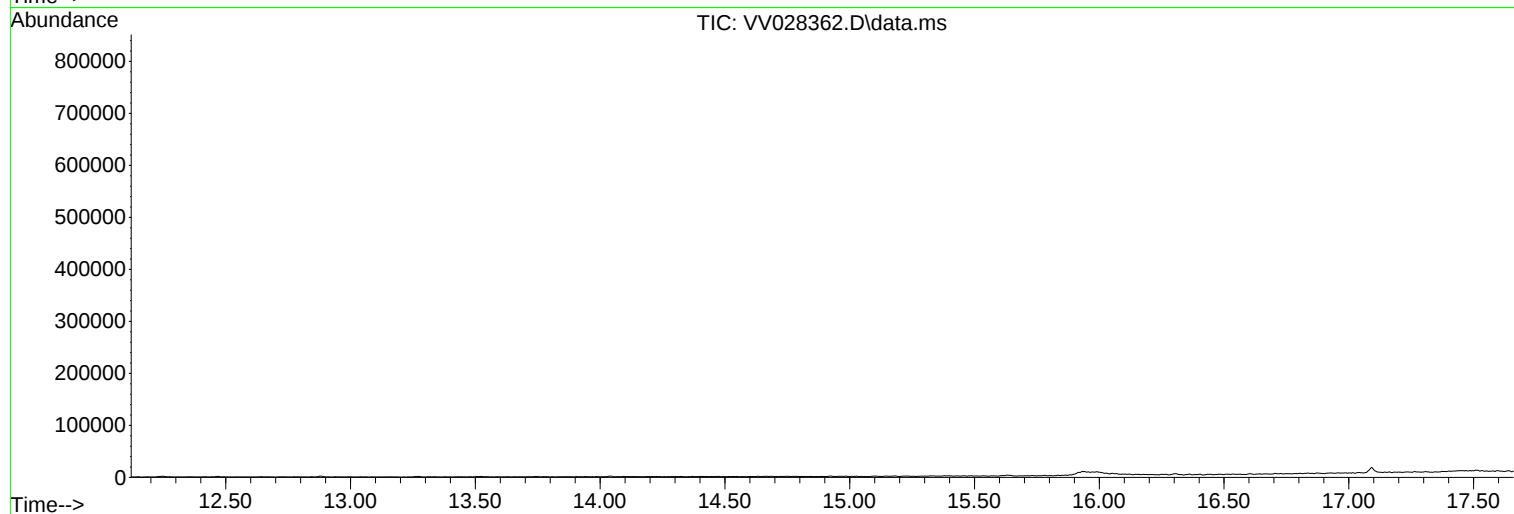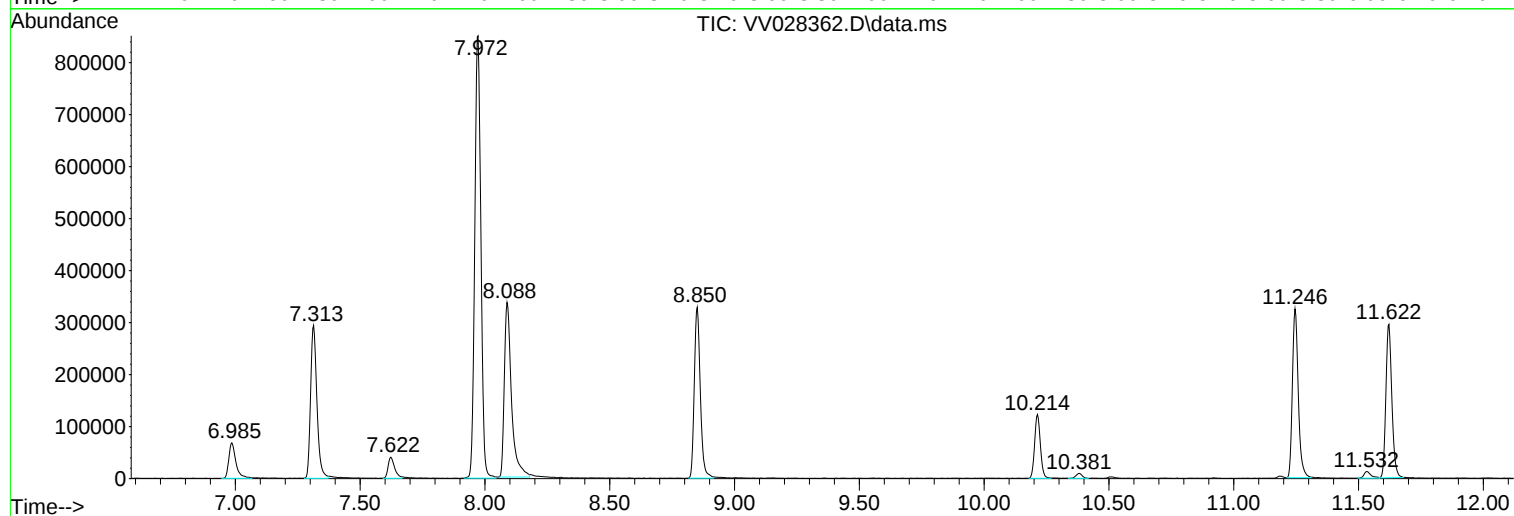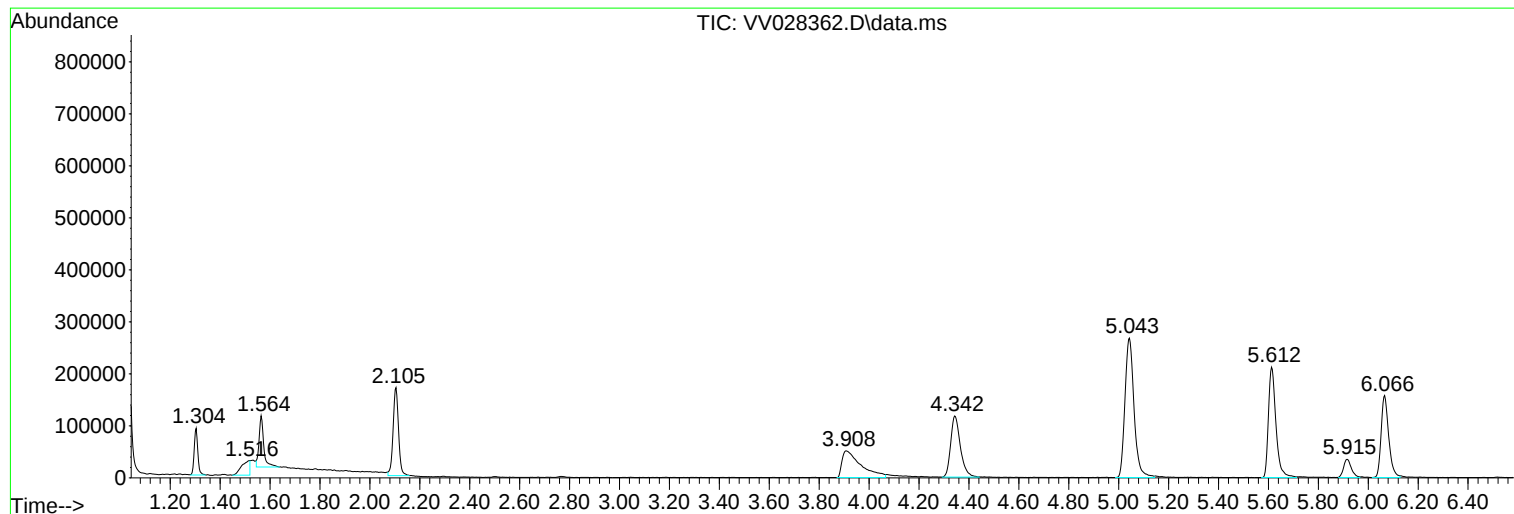

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028362.D
Acq On : 05 Oct 2022 12:45
Operator : SY/MD
Sample : N4899-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028362.D
Acq On : 05 Oct 2022 12:45
Operator : SY/MD
Sample : N4899-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc