

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028370.D
 Acq On : 05 Oct 2022 15:51
 Operator : SY/MD
 Sample : N4866-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFP7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	79404	82307	13.33%	1.562%
2	1.523	132	150	155	rVV	26825	86183	13.96%	1.636%
3	1.565	157	163	175	rVB	85755	112097	18.15%	2.128%
4	2.105	322	331	345	rVB	147251	219092	35.48%	4.159%
5	3.918	881	895	926	rBV2	35938	178870	28.96%	3.395%
6	4.343	1009	1027	1053	rBV	107678	275941	44.68%	5.238%
7	5.043	1228	1245	1276	rBV2	244157	617567	100.00%	11.723%
8	5.613	1410	1422	1457	rBV	205967	434467	70.35%	8.247%
9	6.066	1546	1563	1588	rBV	142551	304211	49.26%	5.775%
10	6.986	1834	1849	1869	rBV	62351	120703	19.54%	2.291%
11	7.314	1937	1951	1973	rBV	261851	470874	76.25%	8.938%
12	7.622	2038	2047	2065	rBV2	34997	66250	10.73%	1.258%
13	7.937	2135	2145	2155	rBV2	8876	15206	2.46%	0.289%
14	8.088	2182	2192	2226	rBV	261242	556522	90.12%	10.564%
15	8.850	2418	2429	2454	rBV	322043	546559	88.50%	10.375%
16	10.214	2840	2853	2869	rBV	112886	180912	29.29%	3.434%
17	10.381	2891	2905	2917	rBV2	20792	34275	5.55%	0.651%
18	11.246	3163	3174	3197	rBV	319529	517208	83.75%	9.818%
19	11.532	3254	3263	3273	rBV6	4878	9264	1.50%	0.176%
20	11.622	3279	3291	3319	rVB	264304	432077	69.96%	8.202%
21	12.249	3474	3486	3496	rBV2	4339	7394	1.20%	0.140%




Sum of corrected areas: 5267979

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028370.D
Acq On : 05 Oct 2022 15:51
Operator : SY/MD
Sample : N4866-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

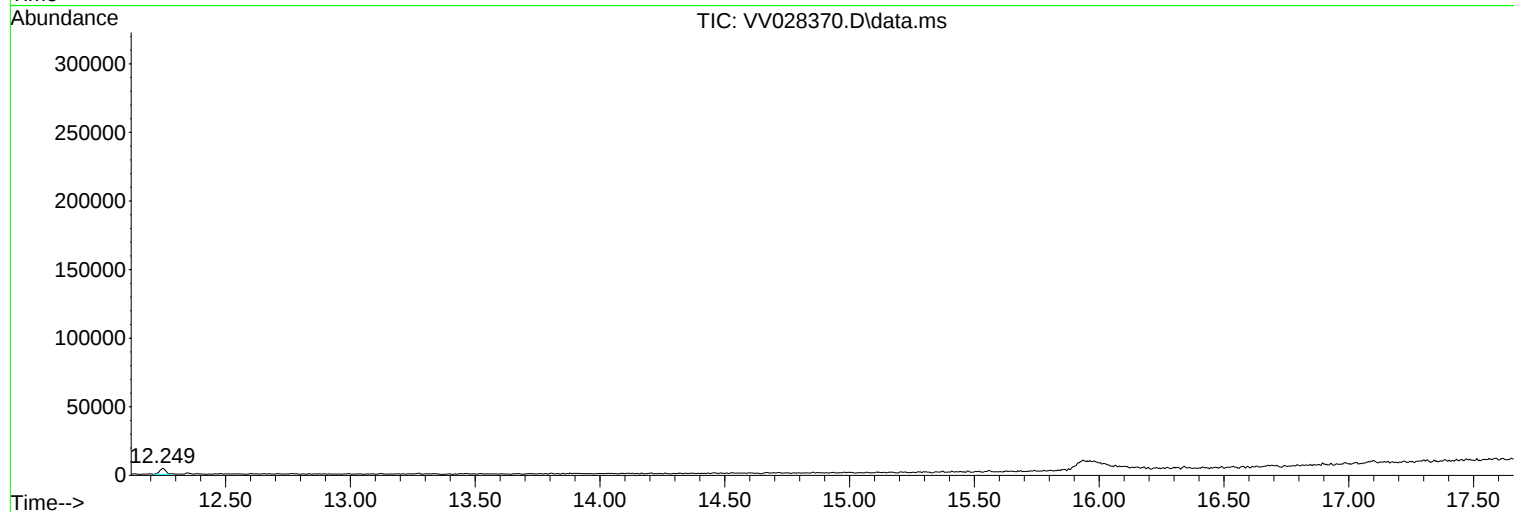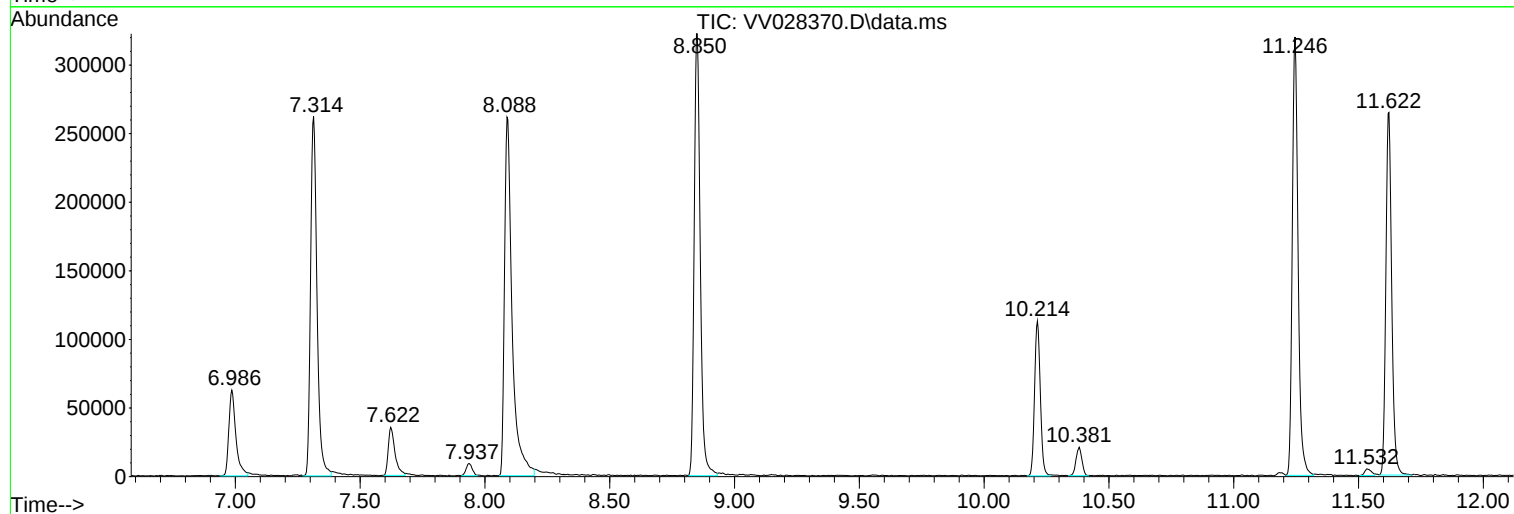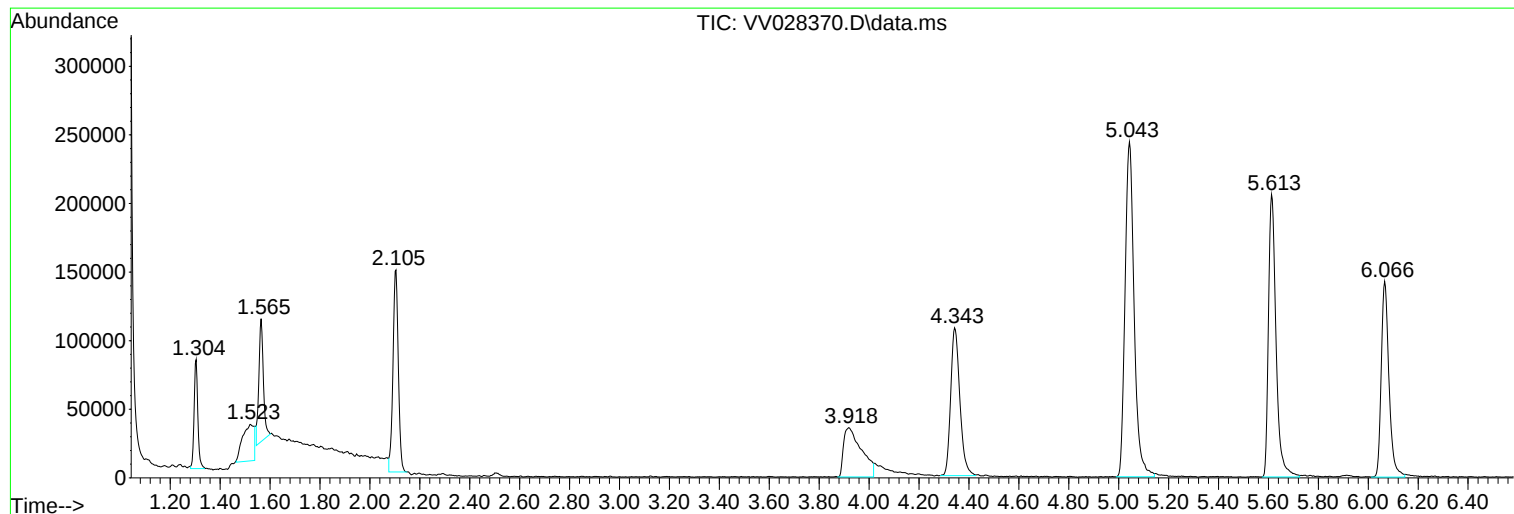

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028370.D
Acq On : 05 Oct 2022 15:51
Operator : SY/MD
Sample : N4866-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028370.D
Acq On : 05 Oct 2022 15:51
Operator : SY/MD
Sample : N4866-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc