

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028374.D
 Acq On : 05 Oct 2022 17:23
 Operator : SY/MD
 Sample : N4872-09DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXFX3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	74876	77386	5.71%	1.181%
2	1.568	140	164	174	rBV2	91166	156542	11.54%	2.389%
3	2.105	322	331	359	rVB	150712	239654	17.67%	3.657%
4	2.506	444	456	469	rVB2	12612	21620	1.59%	0.330%
5	3.924	878	897	943	rBV3	50178	305160	22.50%	4.657%
6	4.346	1010	1028	1051	rBV	113562	285674	21.07%	4.360%
7	5.047	1230	1246	1271	rBV2	252454	628100	46.32%	9.586%
8	5.616	1410	1423	1453	rBV	221197	454129	33.49%	6.931%
9	6.069	1549	1564	1588	rBV	147480	312564	23.05%	4.770%
10	6.985	1835	1849	1866	rBV	61802	118749	8.76%	1.812%
11	7.313	1940	1951	1976	rBV	266688	482736	35.60%	7.367%
12	7.625	2035	2048	2065	rBV2	34285	65898	4.86%	1.006%
13	8.091	2183	2193	2224	rBV	255945	545575	40.23%	8.326%
14	8.850	2418	2429	2459	rBV	342276	603387	44.50%	9.209%
15	10.214	2842	2853	2871	rBV	111051	176529	13.02%	2.694%
16	11.178	3143	3153	3164	rBV2	143452	231458	17.07%	3.532%
17	11.249	3164	3175	3177	rBV	368305	491343	36.24%	7.499%
18	11.638	3279	3296	3318	rBV2	636605	1355983	100.00%	20.694%




Sum of corrected areas: 6552487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028374.D
Acq On : 05 Oct 2022 17:23
Operator : SY/MD
Sample : N4872-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

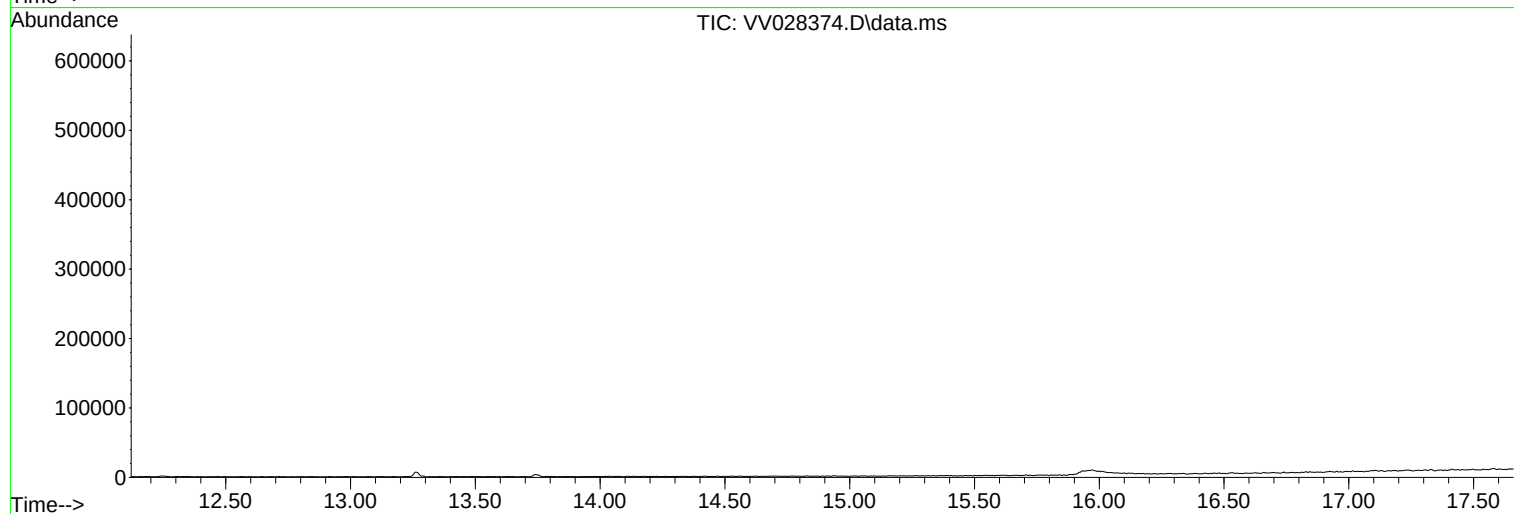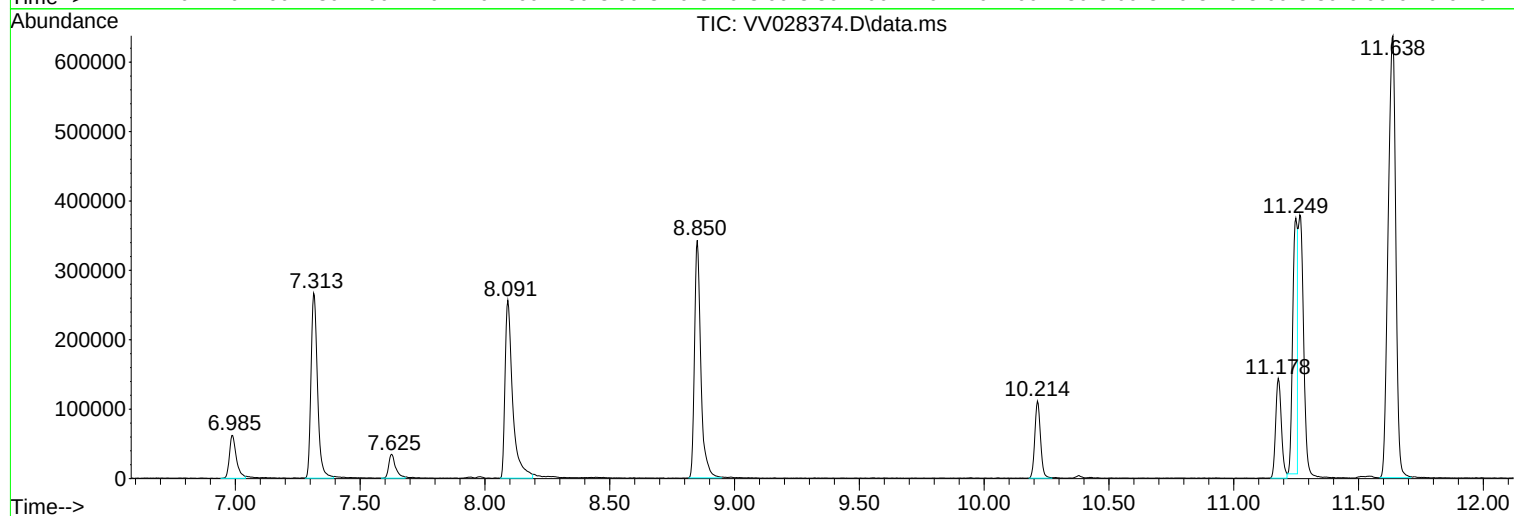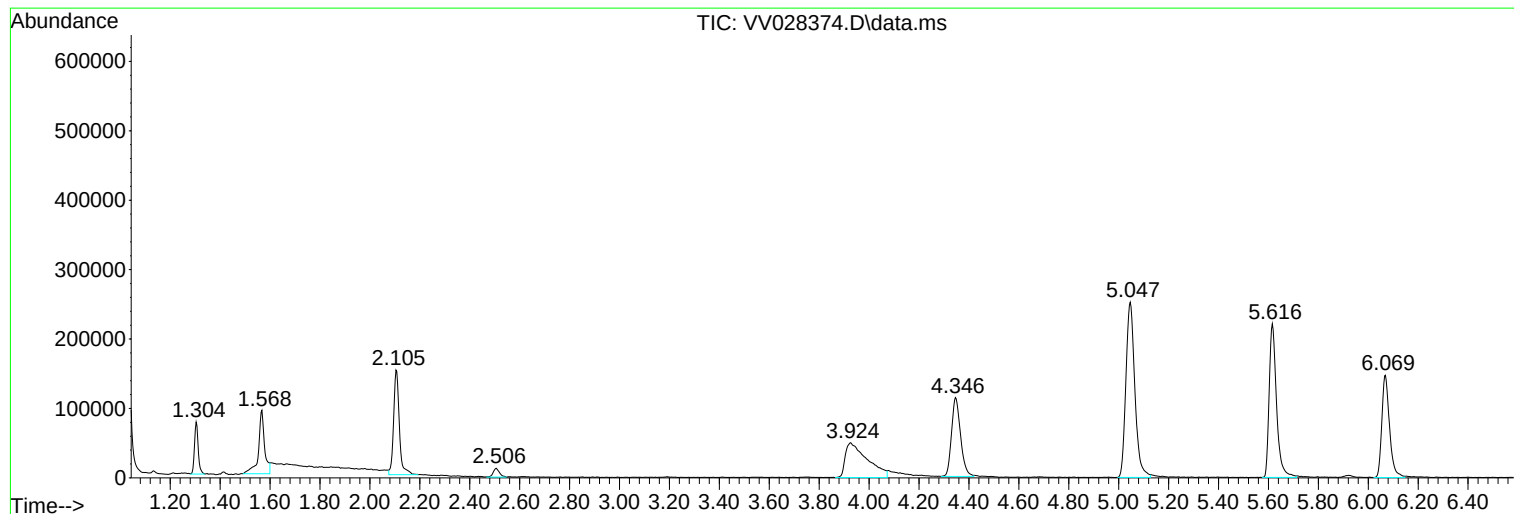

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028374.D
Acq On : 05 Oct 2022 17:23
Operator : SY/MD
Sample : N4872-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
Data File : VV028374.D
Acq On : 05 Oct 2022 17:23
Operator : SY/MD
Sample : N4872-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXFX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc