
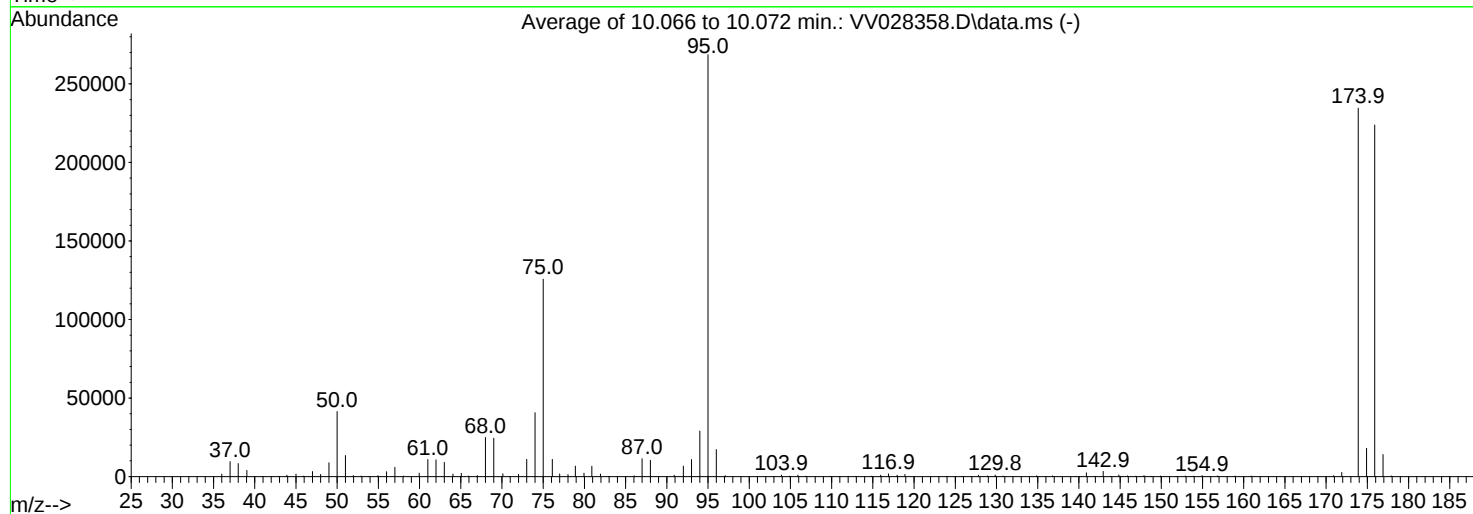


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100522\
 Data File : VV028358.D
 Acq On : 05 Oct 2022 09:09
 Operator : SY/MD
 Sample : BFB383
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB383

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 04 02:28:45 2022

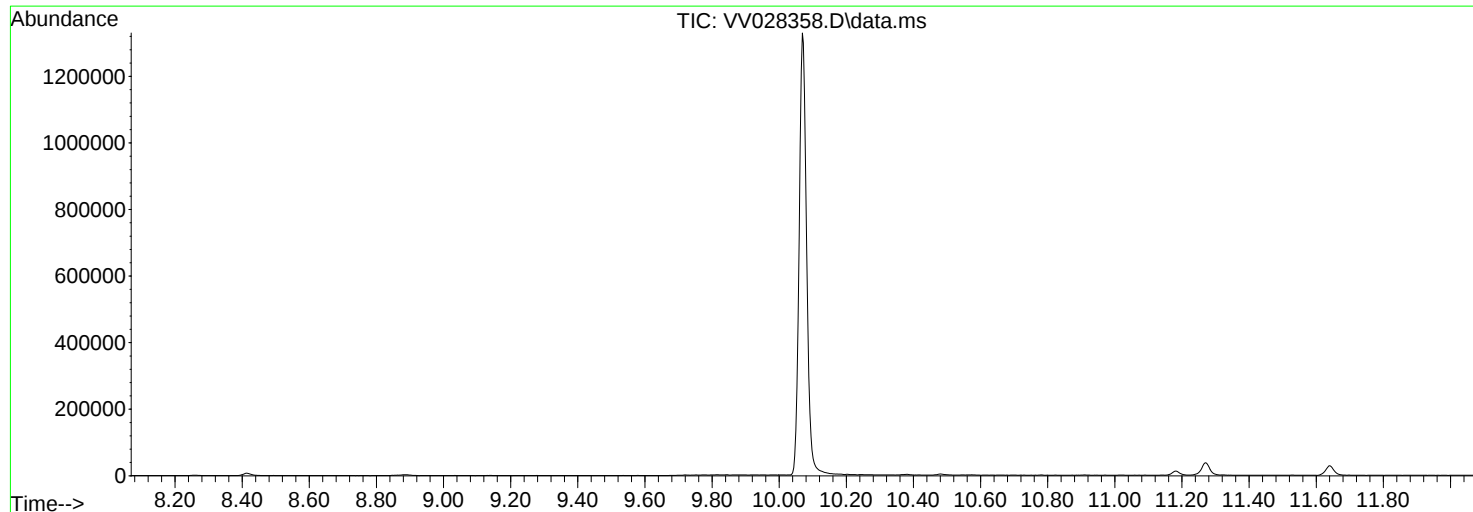

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	41427	PASS
75	95	30	80	46.8	125653	PASS
95	95	100	100	100.0	268565	PASS
96	95	5	9	6.4	17203	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.4	234603	PASS
175	174	5	9	7.7	17960	PASS
176	174	95	105	95.4	223915	PASS
177	176	5	10	6.3	14014	PASS

m/z	Abundance
36.00	1260.0
37.00	104.0
38.00	536.0
40.00	326.0
43.90	389.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
36.00	2905.0
37.00	9229.0
38.00	8922.0
39.10	3894.0
39.90	445.0
40.90	188.0
42.90	201.0
44.00	1191.0
45.00	1608.0
46.00	399.0
47.00	3109.0
48.00	1370.0
49.00	8263.0
50.00	39656.0
51.00	12736.0
51.90	534.0
52.90	286.0
53.80	144.0
54.90	535.0
56.00	3051.0
57.00	5415.0
58.10	343.0
59.00	108.0
60.00	2050.0
61.00	10535.0
62.00	10328.0
63.00	8861.0
64.10	1484.0
65.10	2003.0
66.00	312.0
67.00	681.0
68.00	23624.0
69.00	23192.0
70.10	1703.0
72.00	1484.0
73.00	10659.0
74.00	38536.0
75.00	121112.0
76.10	10492.0
77.00	1759.0
78.00	1312.0
78.90	6439.0
80.00	2080.0
80.90	6304.0
81.90	1476.0
82.90	158.0
86.00	365.0
87.00	10666.0
88.00	9887.0
90.90	854.0
92.00	6530.0
93.00	10218.0
94.00	27296.0
95.00	255680.0
96.00	16744.0
97.10	501.0
103.90	985.0
104.90	271.0
105.90	967.0
107.00	178.0
109.80	149.0
111.00	195.0
112.00	104.0
112.90	164.0
114.90	242.0
115.90	890.0
116.90	1671.0
117.90	806.0
118.90	1328.0
123.90	187.0
126.90	105.0
127.80	890.0
128.90	384.0
129.90	959.0
130.80	363.0
134.80	432.0
136.80	452.0
139.60	174.0
140.90	2262.0
142.00	343.0
142.90	3192.0
143.80	146.0
144.90	1092.0
145.90	564.0
146.90	246.0
147.90	607.0
148.70	211.0
149.90	284.0
151.90	151.0
152.90	236.0
153.90	263.0
154.90	656.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

155.90	103.0
156.90	430.0
158.90	306.0
160.90	351.0
170.90	563.0
171.90	2362.0
173.90	219072.0
174.90	17224.0
175.90	208704.0
176.90	13448.0
177.90	528.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
36.00	2875.0
37.00	10054.0
38.00	9161.0
39.00	4157.0
39.90	468.0
40.90	169.0
42.10	107.0
42.90	212.0
44.00	1293.0
45.00	1643.0
46.00	402.0
47.00	3397.0
48.00	1485.0
49.00	9219.0
50.00	42904.0
51.00	13916.0
52.00	660.0
52.90	356.0
53.80	111.0
55.00	590.0
56.00	3263.0
57.00	6039.0
58.00	340.0
59.00	119.0
59.90	2314.0
61.00	11381.0
62.00	11112.0
63.00	9280.0
64.10	1713.0
65.10	2116.0
65.90	362.0
67.00	733.0
68.00	25928.0
69.00	25368.0
70.10	1941.0
72.00	1434.0
73.00	11334.0
74.00	42408.0
75.00	130520.0
76.10	11383.0
77.00	1783.0
78.00	1389.0
78.90	6895.0
79.90	2212.0
80.90	6875.0
81.90	1641.0
82.90	147.0
86.00	467.0
87.00	11723.0
88.00	10701.0
90.90	928.0
92.00	6909.0
93.00	11370.0
94.00	29864.0
95.00	278208.0
96.00	17736.0
97.10	593.0
103.90	1041.0
104.90	282.0
105.90	1024.0
106.80	207.0
109.80	170.0
110.90	200.0
112.00	161.0
113.00	179.0
114.80	220.0
116.00	897.0
116.90	1701.0
118.00	869.0
118.90	1353.0
124.00	210.0
125.80	147.0
127.80	934.0
128.90	453.0
129.80	1057.0
130.80	390.0
134.80	482.0
136.80	533.0
139.60	171.0
140.10	231.0
140.90	2476.0
141.90	317.0
143.00	3466.0
143.80	217.0
144.80	1174.0
145.90	545.0
146.90	265.0
147.90	707.0
148.70	229.0
149.90	343.0
151.80	155.0
152.90	349.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

153.90	349.0
154.90	686.0
155.90	112.0
156.90	490.0
159.00	353.0
160.90	356.0
170.90	597.0
171.90	2720.0
173.90	243712.0
174.90	18752.0
175.90	232256.0
176.90	14545.0
177.90	562.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
35.00	348.0
36.00	2732.0
37.00	9678.0
38.00	8487.0
39.00	3861.0
39.90	422.0
42.10	116.0
42.90	190.0
43.90	1351.0
45.00	1570.0
45.90	351.0
47.00	3281.0
48.00	1397.0
49.00	9102.0
50.00	41720.0
51.00	13694.0
52.00	683.0
52.90	329.0
55.00	654.0
56.00	3108.0
57.00	6044.0
58.00	302.0
59.90	2222.0
61.00	10634.0
62.00	10663.0
63.00	8815.0
64.00	1685.0
65.00	2101.0
65.90	363.0
67.00	655.0
68.00	25112.0
69.00	24776.0
70.10	1844.0
70.90	113.0
72.00	1266.0
73.00	10818.0
74.00	41288.0
75.00	125328.0
76.10	10922.0
77.00	1589.0
78.00	1242.0
78.90	6594.0
79.90	2149.0
80.90	6614.0
82.00	1589.0
83.00	131.0
86.10	480.0
87.00	11683.0
88.00	10572.0
90.90	861.0
92.00	6752.0
93.00	10995.0
94.00	29848.0
95.00	271808.0
96.00	17128.0
97.10	639.0
103.00	108.0
103.90	963.0
104.90	296.0
105.90	972.0
106.80	265.0
109.90	157.0
110.80	176.0
112.00	165.0
113.00	171.0
114.90	206.0
116.00	752.0
116.90	1596.0
118.00	864.0
118.90	1303.0
124.00	165.0
125.80	188.0
127.80	869.0
128.90	500.0
129.80	1001.0
130.80	376.0
134.90	465.0
136.80	536.0
139.70	127.0
140.90	2446.0
141.90	278.0
143.00	3309.0
143.80	232.0
144.80	1076.0
145.90	465.0
146.90	190.0
147.90	717.0
148.80	206.0
149.90	345.0
151.70	151.0
152.90	383.0
153.90	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

155.00	678.0
155.90	102.0
156.80	468.0
159.00	372.0
160.90	315.0
170.90	516.0
171.90	2824.0
173.90	241024.0
174.90	17904.0
175.90	230784.0
176.90	14048.0
177.90	492.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383