

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100719\
 Data File : VV013051.D
 Acq On : 07 Oct 2019 12:15
 Operator : SY/MD
 Sample : VV1007SBL01
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Quant Time: Oct 08 17:13:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 08 16:45:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	767749	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	752519	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	366479	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	241718	20.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.16%
7) Chloroethane-d5	1.58	69	225231	23.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.56%
10) 1,1-Dichloroethene-d2	2.13	63	340068	17.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.68%
20) 2-Butanone-d5	3.93	46	218584	53.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.28%
24) Chloroform-d	4.40	84	504513	23.92	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.68%
26) 1,2-Dichloroethane-d4	5.08	65	300166	24.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.92%
29) Benzene-d6	5.10	84	1037139	24.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.76%
33) 1,2-Dichloropropane-d6	6.11	67	331339	25.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.64%
37) Toluene-d8	7.36	98	924340	24.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.92%
38) trans-1,3-Dichloropropene-	7.66	79	135293	24.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.04%
39) 2-Hexanone-d5	8.13	63	150999	56.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.96%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	309072	24.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.84%
61) 1,2-Dichlorobenzene-d4	11.67	152	382958	26.90	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	11339	2.594 ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100719\
Data File : VV013051.D
Acq On : 07 Oct 2019 12:15
Operator : SY/MD
Sample : VV1007SBL01
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK74

Quant Time: Oct 08 17:13:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 08 16:45:23 2019
Response via : Initial Calibration

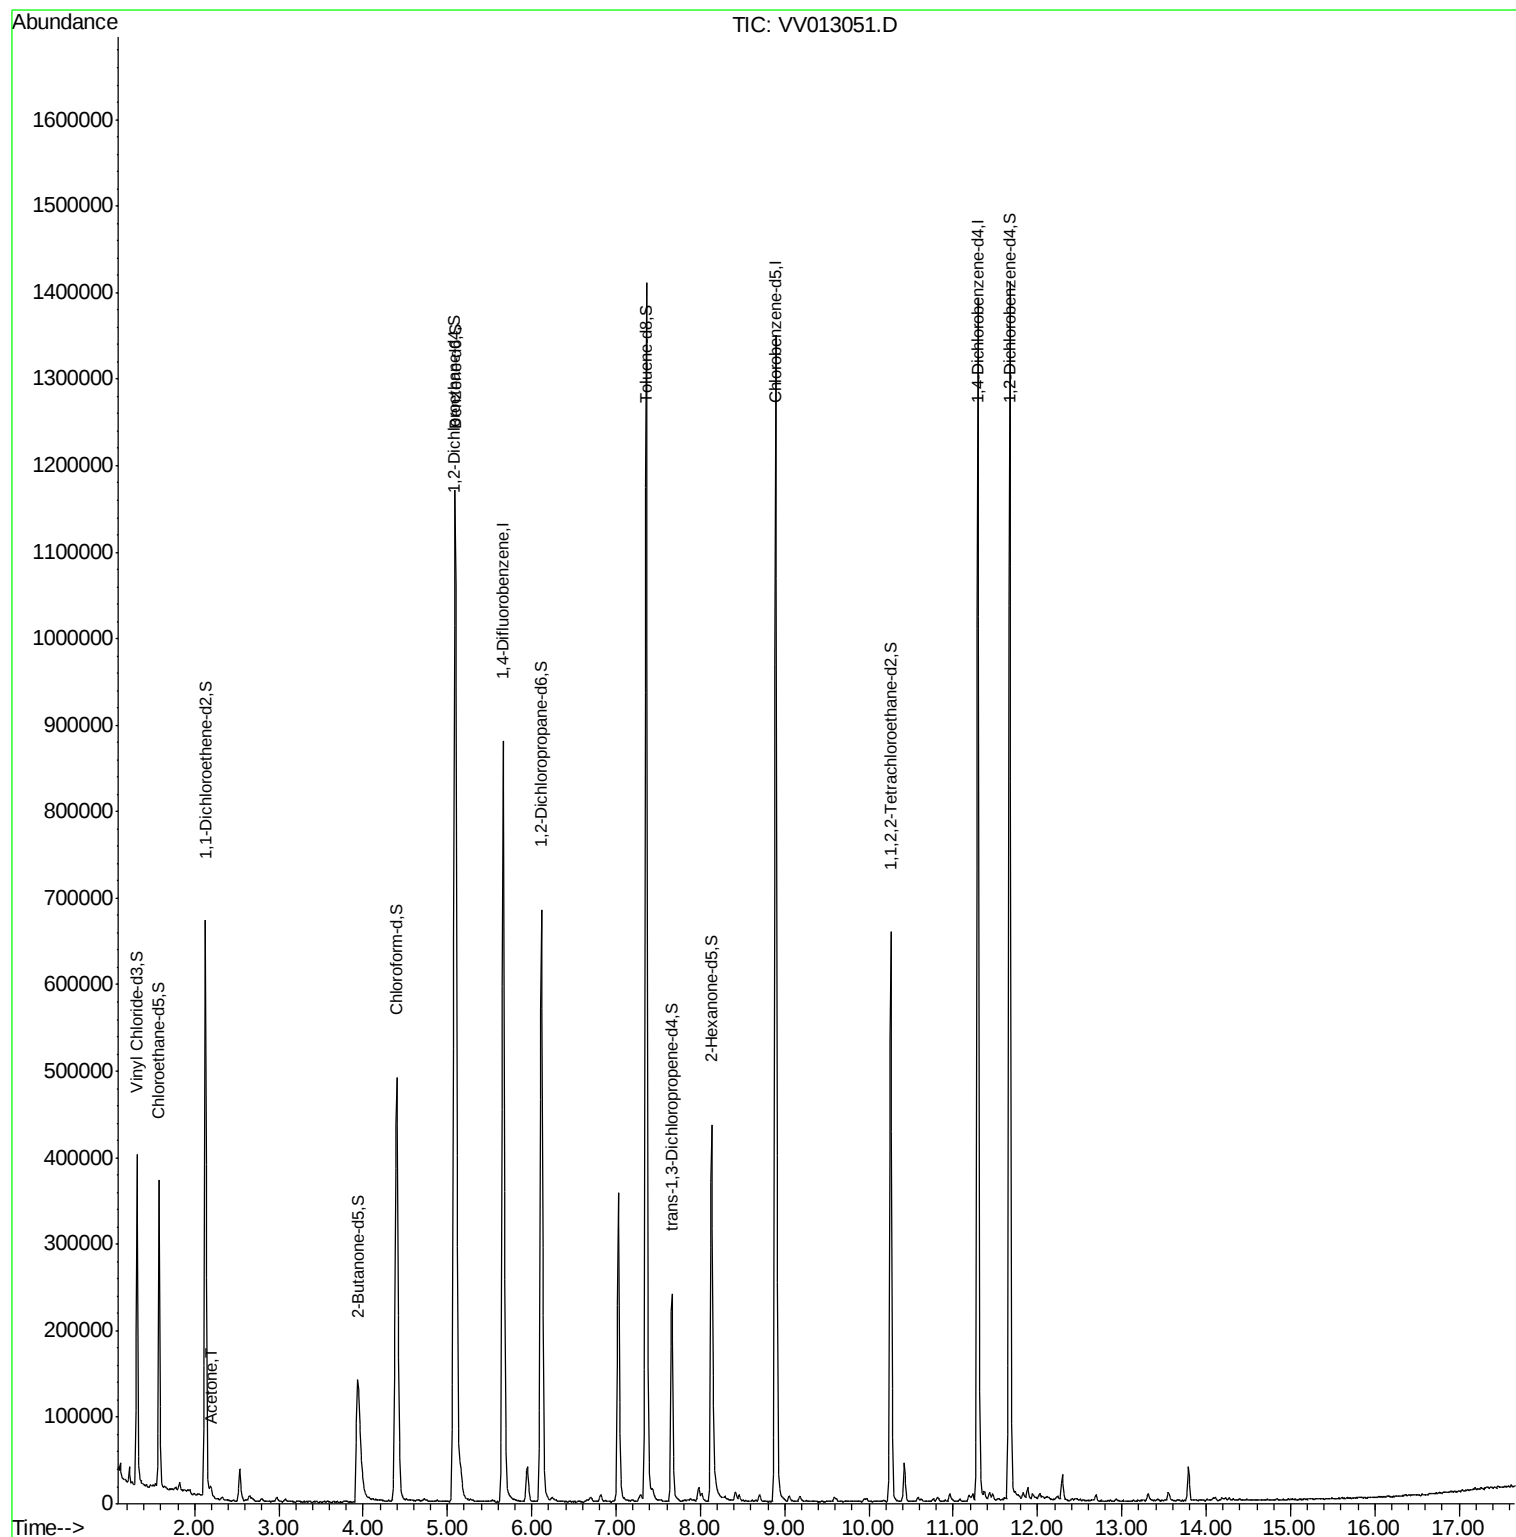

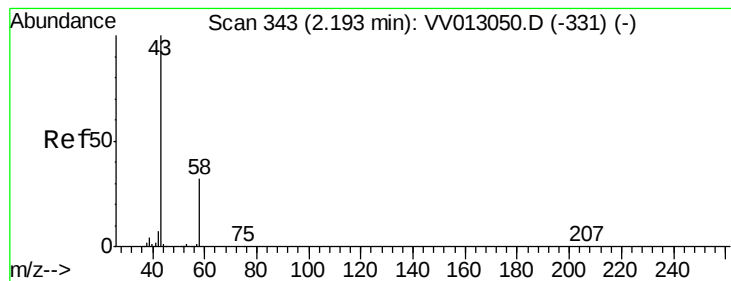

#13

Acetone

Concen: 2.594 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.01 min

Lab File: VV013051.D

Acq: 07 Oct 2019 12:15

Instrument :

MSVOA_V

ClientSampleId :

VBLK74

Tot Ion: 43 Resp: 11339

Ion Ratio Lower Upper

43 100

58 17.5 0.0 65.0

