


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100719\
Data File : VV013049.D
Acq On : 07 Oct 2019 08:59
Operator : SY/MD
Sample : BFB67
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Title : VOC Analysis
Last Update : Tue Oct 08 16:45:23 2019

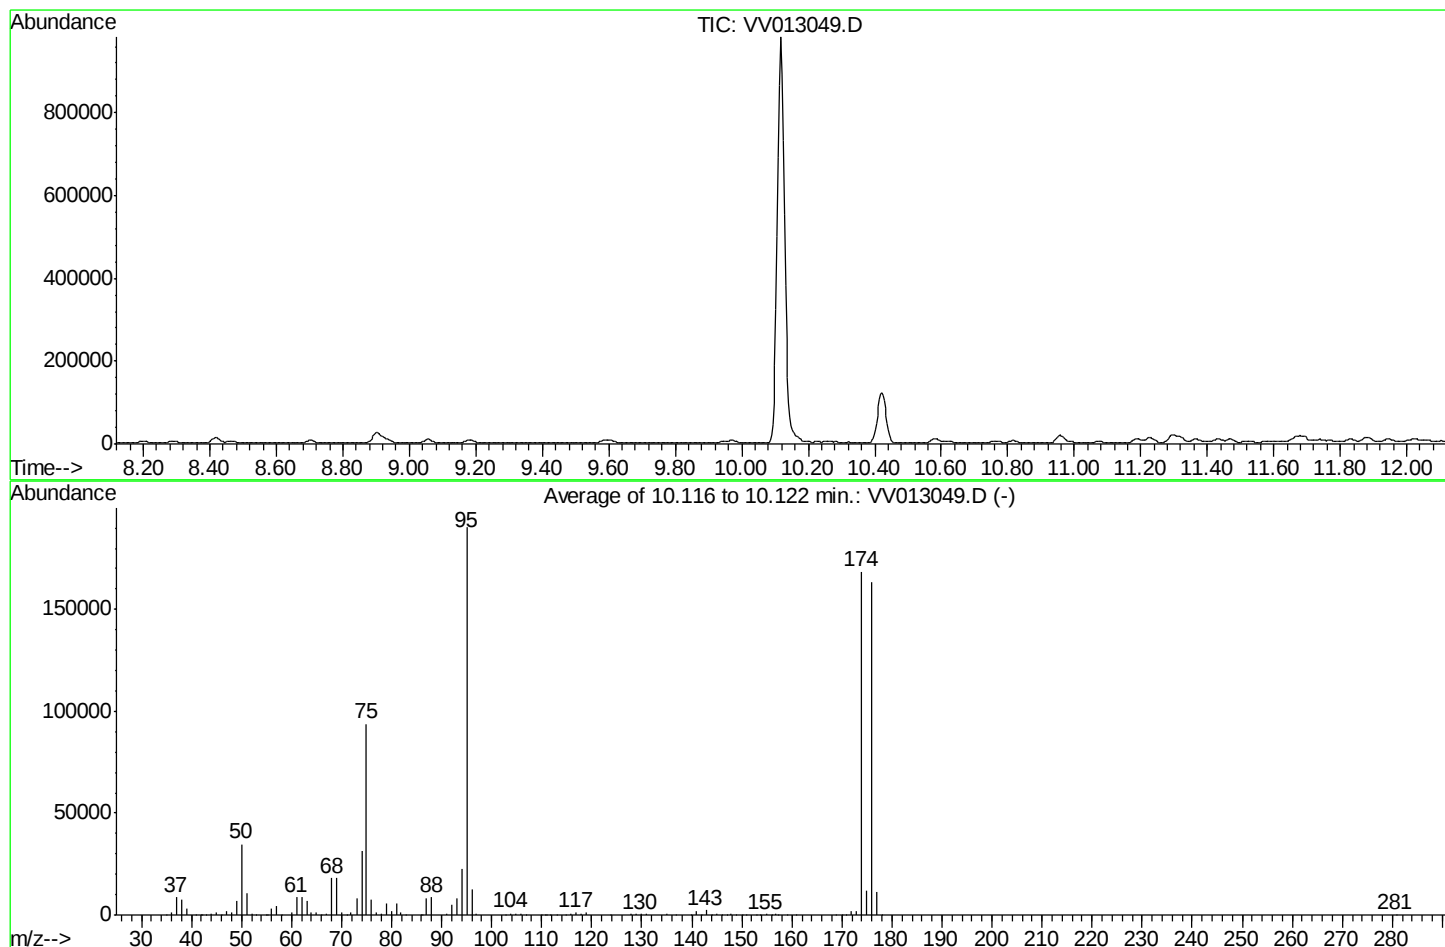

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	34560	PASS
75	95	30	80	49.3	93874	PASS
95	95	100	100	100.0	190272	PASS
96	95	5	9	6.5	12308	PASS
173	174	0.00	2	1.0	1768	PASS
174	95	50	120	88.7	168682	PASS
175	174	5	9	7.2	12178	PASS
176	174	95	101	96.8	163221	PASS
177	176	5	9	6.8	11068	PASS

m/z	Abundance
35.00	138.0
36.00	1474.0
37.00	9202.0
38.00	7891.0
39.10	3700.0
40.00	948.0
40.80	180.0
43.10	209.0
44.00	1846.0
45.00	1573.0
45.90	231.0
47.00	2208.0
47.90	1315.0
49.00	7738.0
50.00	36376.0
51.00	11462.0
52.00	537.0
53.00	117.0
54.90	386.0
56.10	3134.0
57.00	4637.0
58.00	161.0
60.00	1537.0
61.00	9167.0
62.00	9224.0
63.00	7225.0
64.00	1117.0
65.00	1608.0
66.10	163.0
66.90	631.0
68.00	18880.0
69.00	18480.0
70.00	1554.0
71.90	1119.0
73.00	8227.0
74.00	32960.0
75.00	98064.0
76.00	8336.0
77.10	1154.0
77.90	797.0
78.90	5728.0
80.00	1847.0
80.90	5757.0
81.90	1593.0
82.90	143.0
85.80	204.0
86.10	249.0
86.90	8438.0
87.90	8865.0
90.90	680.0
92.00	5089.0
93.00	8724.0
94.00	23272.0
95.00	196800.0
96.00	13047.0
97.00	471.0
102.80	138.0
103.80	889.0
104.90	379.0
105.90	717.0
106.90	235.0
109.90	101.0
110.90	176.0
111.80	165.0
113.10	144.0
114.90	229.0
115.80	724.0
116.90	1266.0
117.90	671.0
118.90	973.0
123.80	161.0
127.80	582.0
128.90	383.0
129.80	682.0
130.90	333.0
134.90	465.0
136.70	378.0
140.90	1720.0
141.90	320.0
142.90	2456.0
143.90	183.0
144.90	471.0
145.90	335.0
146.90	101.0
147.90	382.0
148.80	161.0
150.00	223.0
150.90	101.0
152.90	121.0
153.70	111.0
154.90	456.0
156.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

156.90	343.0
159.00	261.0
160.90	205.0
170.90	278.0
172.00	1938.0
172.90	1858.0
173.90	169024.0
175.00	12518.0
175.90	162304.0
176.90	11547.0
177.90	315.0
280.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	1615.0
37.00	9048.0
38.00	7493.0
39.00	3705.0
40.00	998.0
40.80	176.0
43.00	197.0
44.00	1910.0
45.00	1563.0
45.90	189.0
47.00	2087.0
47.90	1123.0
49.00	7472.0
50.00	35768.0
51.00	11149.0
52.00	559.0
53.10	127.0
55.10	400.0
56.00	3213.0
57.00	4749.0
58.00	176.0
60.00	1636.0
61.00	8905.0
62.00	9008.0
63.00	7173.0
64.00	1051.0
65.00	1557.0
66.00	159.0
67.00	626.0
68.00	18544.0
69.00	18872.0
70.00	1563.0
71.10	132.0
71.90	1129.0
73.00	8189.0
74.00	32744.0
75.00	97312.0
76.00	8016.0
77.00	1340.0
77.80	887.0
78.90	5511.0
79.90	1686.0
80.90	5755.0
81.90	1482.0
82.90	163.0
85.70	252.0
86.10	242.0
86.90	8175.0
87.90	9034.0
90.90	818.0
92.00	5185.0
93.00	8508.0
94.00	23072.0
95.00	196864.0
96.00	12664.0
97.00	423.0
102.80	137.0
103.90	957.0
104.90	350.0
105.90	747.0
106.90	205.0
110.60	163.0
111.00	167.0
111.80	196.0
113.00	125.0
114.90	238.0
115.80	642.0
116.90	1180.0
117.90	738.0
118.90	1036.0
123.80	224.0
127.90	601.0
128.90	337.0
129.80	629.0
131.00	355.0
135.00	443.0
136.70	340.0
139.80	140.0
140.90	1848.0
141.90	286.0
142.90	2429.0
143.80	162.0
145.00	472.0
145.90	334.0
147.00	115.0
147.90	429.0
148.80	141.0
150.00	264.0
152.90	104.0
153.70	120.0
154.90	459.0
156.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

156.80	334.0
159.00	266.0
160.80	231.0
168.70	106.0
170.90	211.0
172.00	2021.0
172.90	1860.0
173.90	175040.0
175.00	12695.0
175.90	169024.0
176.90	11439.0
177.90	305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	1544.0
37.00	7914.0
38.00	6671.0
39.00	3309.0
39.90	1056.0
40.80	146.0
41.80	111.0
42.20	107.0
42.90	245.0
44.00	1867.0
45.00	1458.0
45.90	167.0
47.00	1886.0
48.00	985.0
49.00	6474.0
50.00	31536.0
51.00	9790.0
52.00	558.0
52.90	130.0
55.10	415.0
56.00	2966.0
57.00	4388.0
58.00	188.0
60.00	1482.0
61.00	8070.0
62.00	7827.0
63.00	6560.0
64.00	906.0
65.00	1350.0
66.00	135.0
67.00	574.0
68.00	16392.0
69.00	17264.0
70.00	1460.0
71.20	155.0
71.90	985.0
73.00	7407.0
74.00	28904.0
75.00	86248.0
76.00	6893.0
77.00	1229.0
77.80	882.0
78.90	4984.0
79.90	1367.0
80.90	5278.0
81.90	1321.0
82.90	149.0
85.70	243.0
86.20	218.0
86.90	7315.0
88.00	8136.0
90.90	835.0
92.00	4822.0
93.00	7478.0
94.00	20696.0
95.00	177152.0
96.00	11215.0
97.00	310.0
102.80	130.0
103.90	902.0
104.90	292.0
105.80	662.0
106.90	168.0
110.60	173.0
111.10	143.0
111.80	197.0
113.00	119.0
114.90	209.0
115.80	558.0
116.90	944.0
117.90	700.0
118.90	991.0
123.80	222.0
127.90	649.0
128.90	304.0
129.80	553.0
131.00	365.0
135.00	382.0
136.80	278.0
139.70	163.0
140.90	1707.0
141.90	194.0
142.90	2213.0
145.00	430.0
145.90	284.0
147.00	148.0
147.90	428.0
148.70	134.0
150.00	234.0
152.80	121.0
153.70	109.0
155.00	439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

156.70	346.0
157.20	182.0
158.90	241.0
160.80	245.0
170.00	106.0
170.70	173.0
171.90	1865.0
172.90	1586.0
173.90	161984.0
175.00	11323.0
175.90	158336.0
176.90	10220.0
178.00	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Scan 2794 (10.074 min): VV013049.D
BFB67

m/z	Abundance
36.70	107.0
39.10	134.0
40.00	1047.0
41.00	118.0
44.00	1192.0
78.10	119.0
87.30	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67