

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028407.D
 Acq On : 07 Oct 2022 15:12
 Operator : SY/MD
 Sample : N4853-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1B0

Quant Time: Oct 08 00:59:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	453250	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	397139	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	192100	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	138541	39.614	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.220%		
7) Chloroethane-d5	1.564	69	118153	42.607	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.220%		
11) 1,1-Dichloroethene-d2	2.101	63	187994	31.584	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.160%		
21) 2-Butanone-d5	3.902	46	296883	96.972	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.970%		
24) Chloroform-d	4.339	84	281881	43.947	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.900%		
26) 1,2-Dichloroethane-d4	5.027	65	193438	46.762	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.520%		
32) Benzene-d6	5.043	84	603472	47.422	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.840%		
36) 1,2-Dichloropropane-d6	6.066	67	198956	47.952	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.900%		
41) Toluene-d8	7.310	98	536888	47.123	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.240%		
43) trans-1,3-Dichloroprop...	7.616	79	98869	46.751	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.500%		
47) 2-Hexanone-d5	8.085	63	216900	96.100	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.100%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	266398	46.920	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.840%		
66) 1,2-Dichlorobenzene-d4	11.615	152	191334	48.069	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.140%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	1961	0.726	ug/L	# 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028407.D
Acq On : 07 Oct 2022 15:12
Operator : SY/MD
Sample : N4853-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1B0

Quant Time: Oct 08 00:59:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 23:51:49 2022
Response via : Initial Calibration

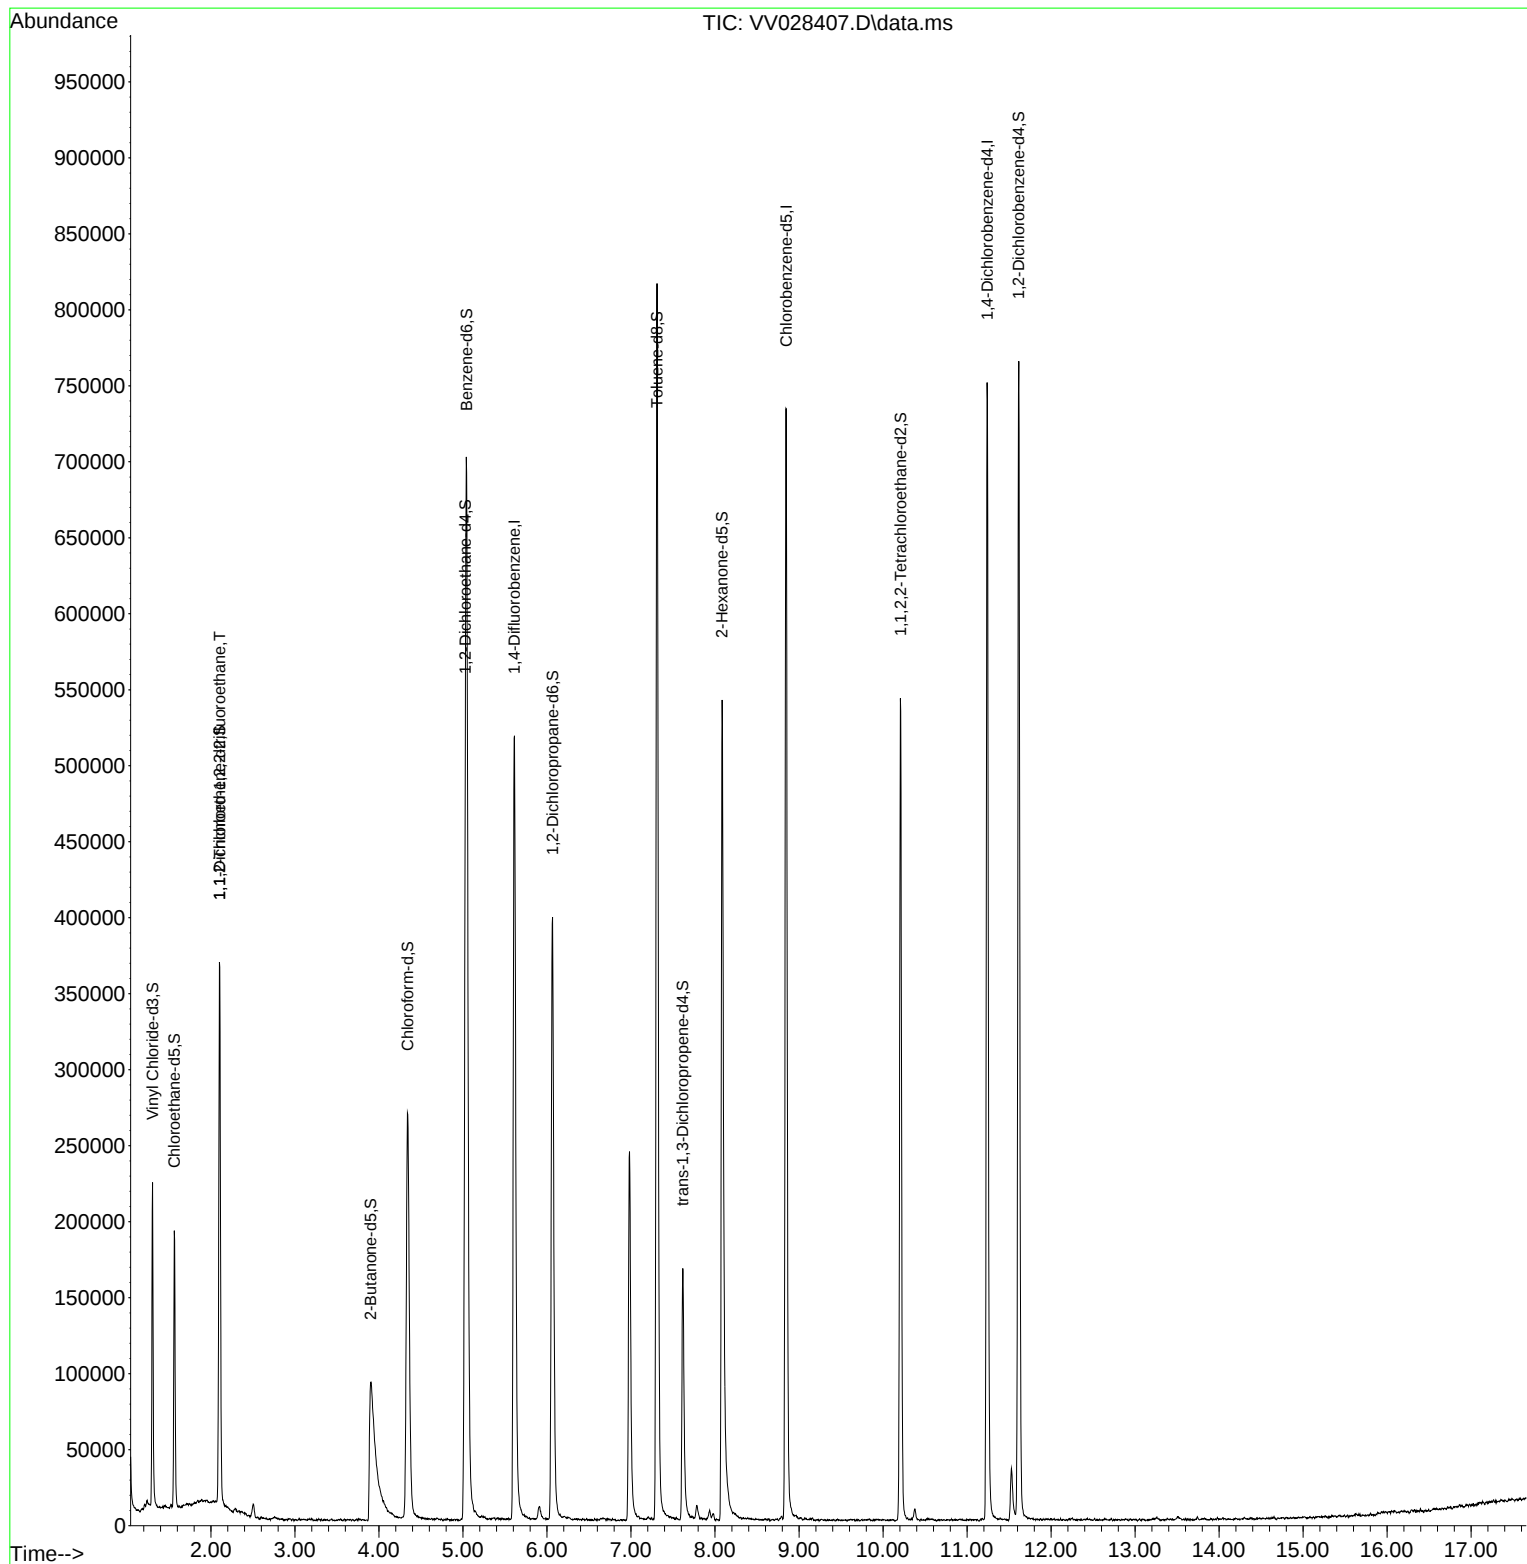

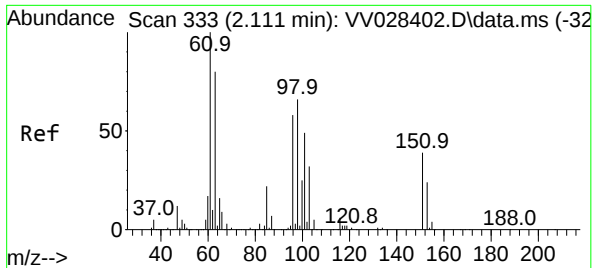

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.726 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV028407.D
 Acq: 07 Oct 2022 15:12

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1B0

Tgt Ion:	101	Resp:	1961
Ion	Ratio	Lower	Upper
101	100		
85	8.1	34.9	52.3#
151	0.0	59.2	88.8#

