

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028409.D
 Acq On : 07 Oct 2022 16:00
 Operator : SY/MD
 Sample : N4890-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 08 00:59:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	432558	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	385907	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	186697	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	136824	40.994	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.980%		
7) Chloroethane-d5	1.564	69	115798	43.755	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.520%		
11) 1,1-Dichloroethene-d2	2.101	63	186190	32.777	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.560%		
21) 2-Butanone-d5	3.896	46	282390	96.650	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.650%		
24) Chloroform-d	4.342	84	280073	45.753	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.500%		
26) 1,2-Dichloroethane-d4	5.027	65	191325	48.464	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.920%		
32) Benzene-d6	5.043	84	592091	47.881	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.760%		
36) 1,2-Dichloropropane-d6	6.066	67	196661	48.778	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.560%		
41) Toluene-d8	7.310	98	530684	47.934	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.860%		
43) trans-1,3-Dichloroprop...	7.616	79	97677	47.531	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.060%		
47) 2-Hexanone-d5	8.085	63	216197	98.576	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.580%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	268451	48.658	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.320%		
66) 1,2-Dichlorobenzene-d4	11.615	152	190766	49.313	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.620%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.619	75	4480	0.862	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028409.D
Acq On : 07 Oct 2022 16:00
Operator : SY/MD
Sample : N4890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 08 00:59:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 23:51:49 2022
Response via : Initial Calibration

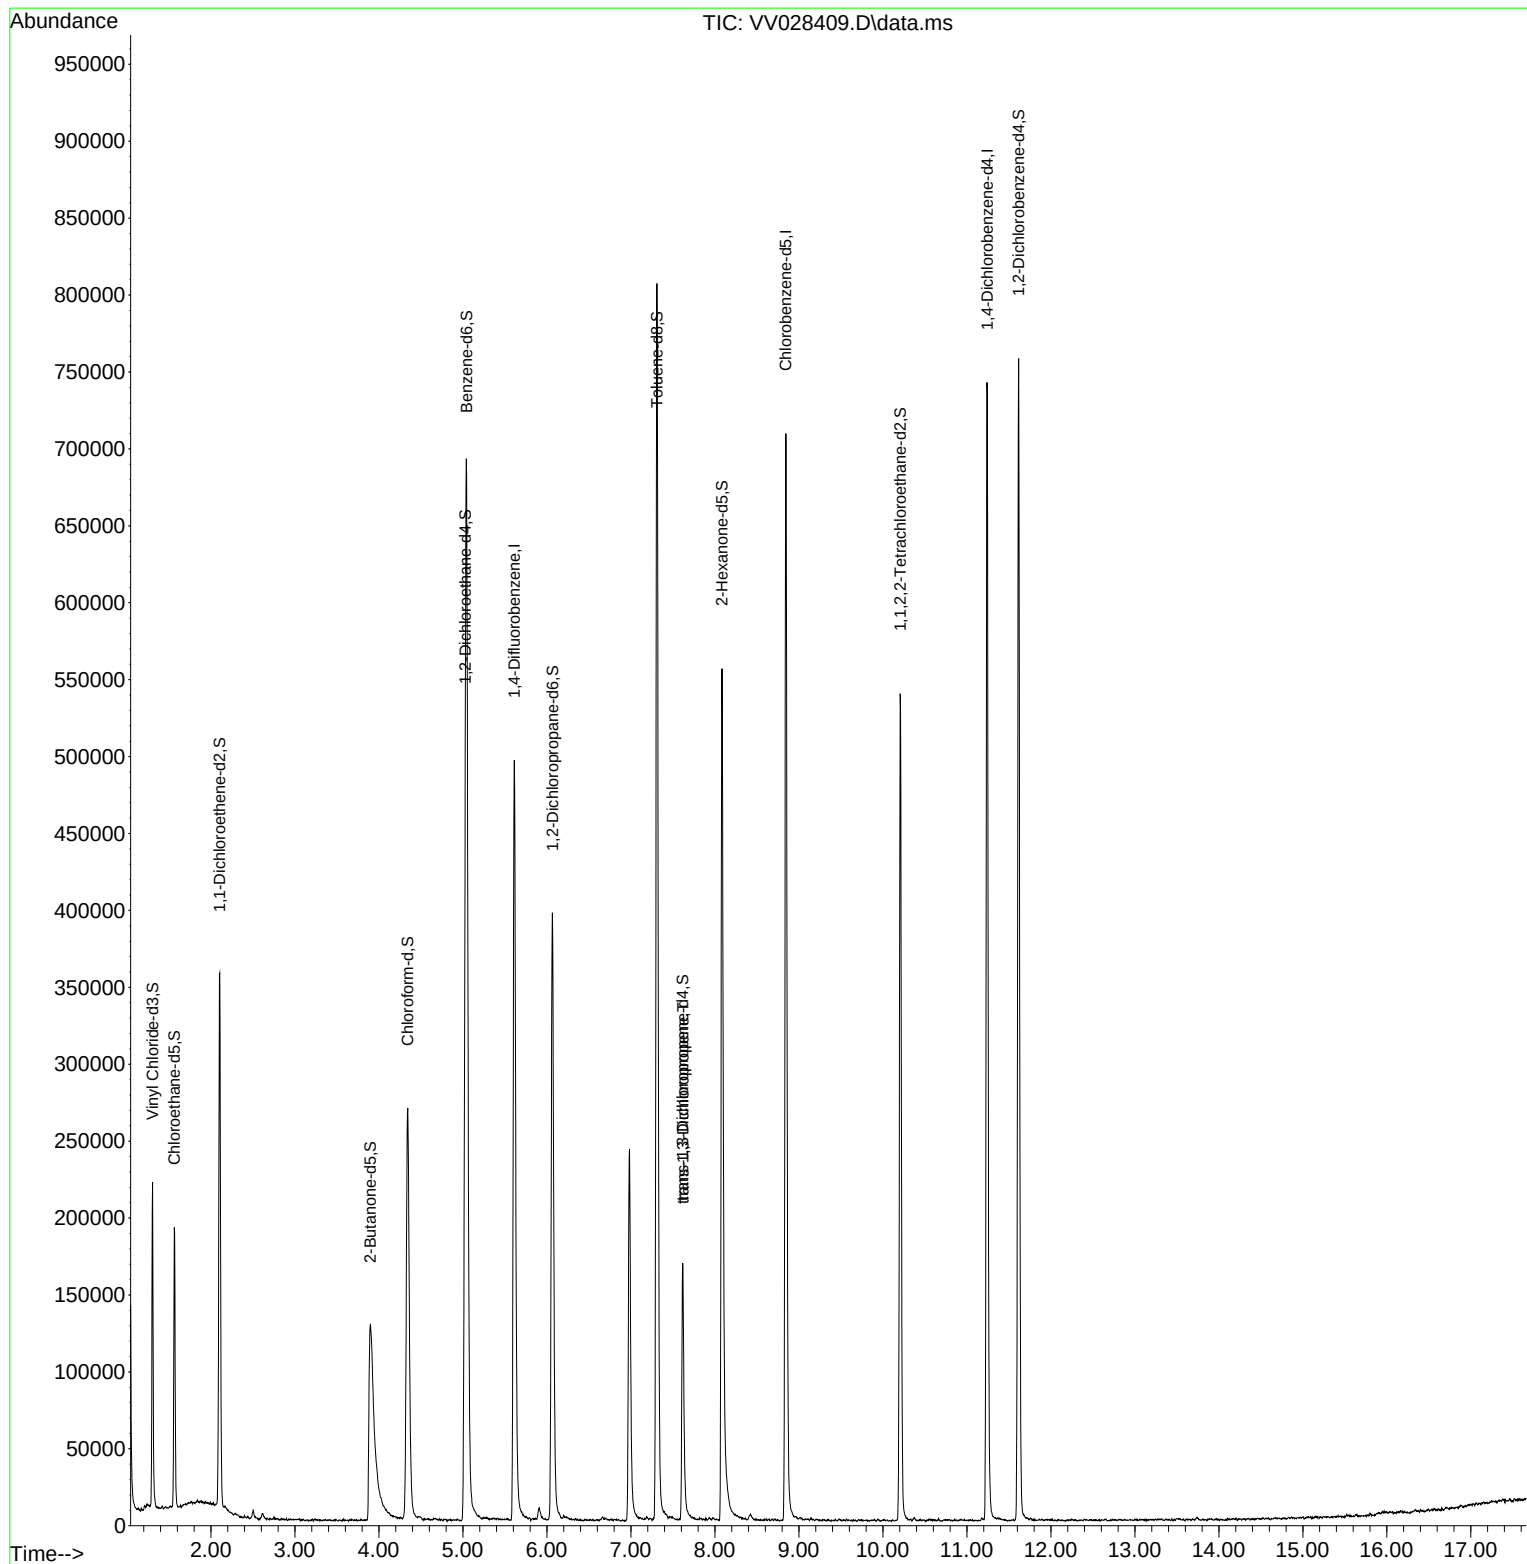

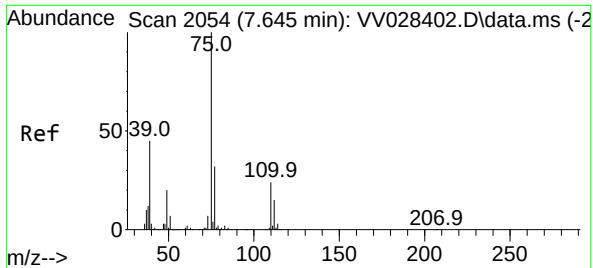

#44
 trans-1,3-Dichloropropene
 Concen: 0.862 ug/L
 RT: 7.619 min Scan# 2046
 Delta R.T. -0.026 min
 Lab File: VV028409.D
 Acq: 07 Oct 2022 16:00

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 4480
 Ion Ratio Lower Upper
 75 100
 77 47.1 21.8 40.4#

