

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028436.D
 Acq On : 08 Oct 2022 03:13
 Operator : SY/MD
 Sample : N4942-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS2

Quant Time: Oct 08 04:01:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 08 02:10:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	365991	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	330465	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	159261	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	89840	31.813	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	63.620%
7) Chloroethane-d5	1.565	69	78878	35.226	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	70.460%
11) 1,1-Dichloroethene-d2	2.102	63	128320	26.699	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	53.400%#
21) 2-Butanone-d5	3.899	46	192330	77.799	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	77.800%
24) Chloroform-d	4.343	84	222615	42.981	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.960%
26) 1,2-Dichloroethane-d4	5.027	65	155943	46.686	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.380%
32) Benzene-d6	5.043	84	466492	44.053	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.100%
36) 1,2-Dichloropropane-d6	6.063	67	154747	44.821	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.640%
41) Toluene-d8	7.310	98	418010	44.091	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.180%
43) trans-1,3-Dichloroprop...	7.616	79	73748	41.908	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.820%
47) 2-Hexanone-d5	8.085	63	163453	87.031	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.030%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	209548	44.354	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.700%
66) 1,2-Dichlorobenzene-d4	11.616	152	154330	46.767	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.540%
Target Compounds						
61) 1,2,3-Trichloropropane	11.239	75	20282	5.982	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028436.D
Acq On : 08 Oct 2022 03:13
Operator : SY/MD
Sample : N4942-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSH2

Quant Time: Oct 08 04:01:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 08 02:10:35 2022
Response via : Initial Calibration

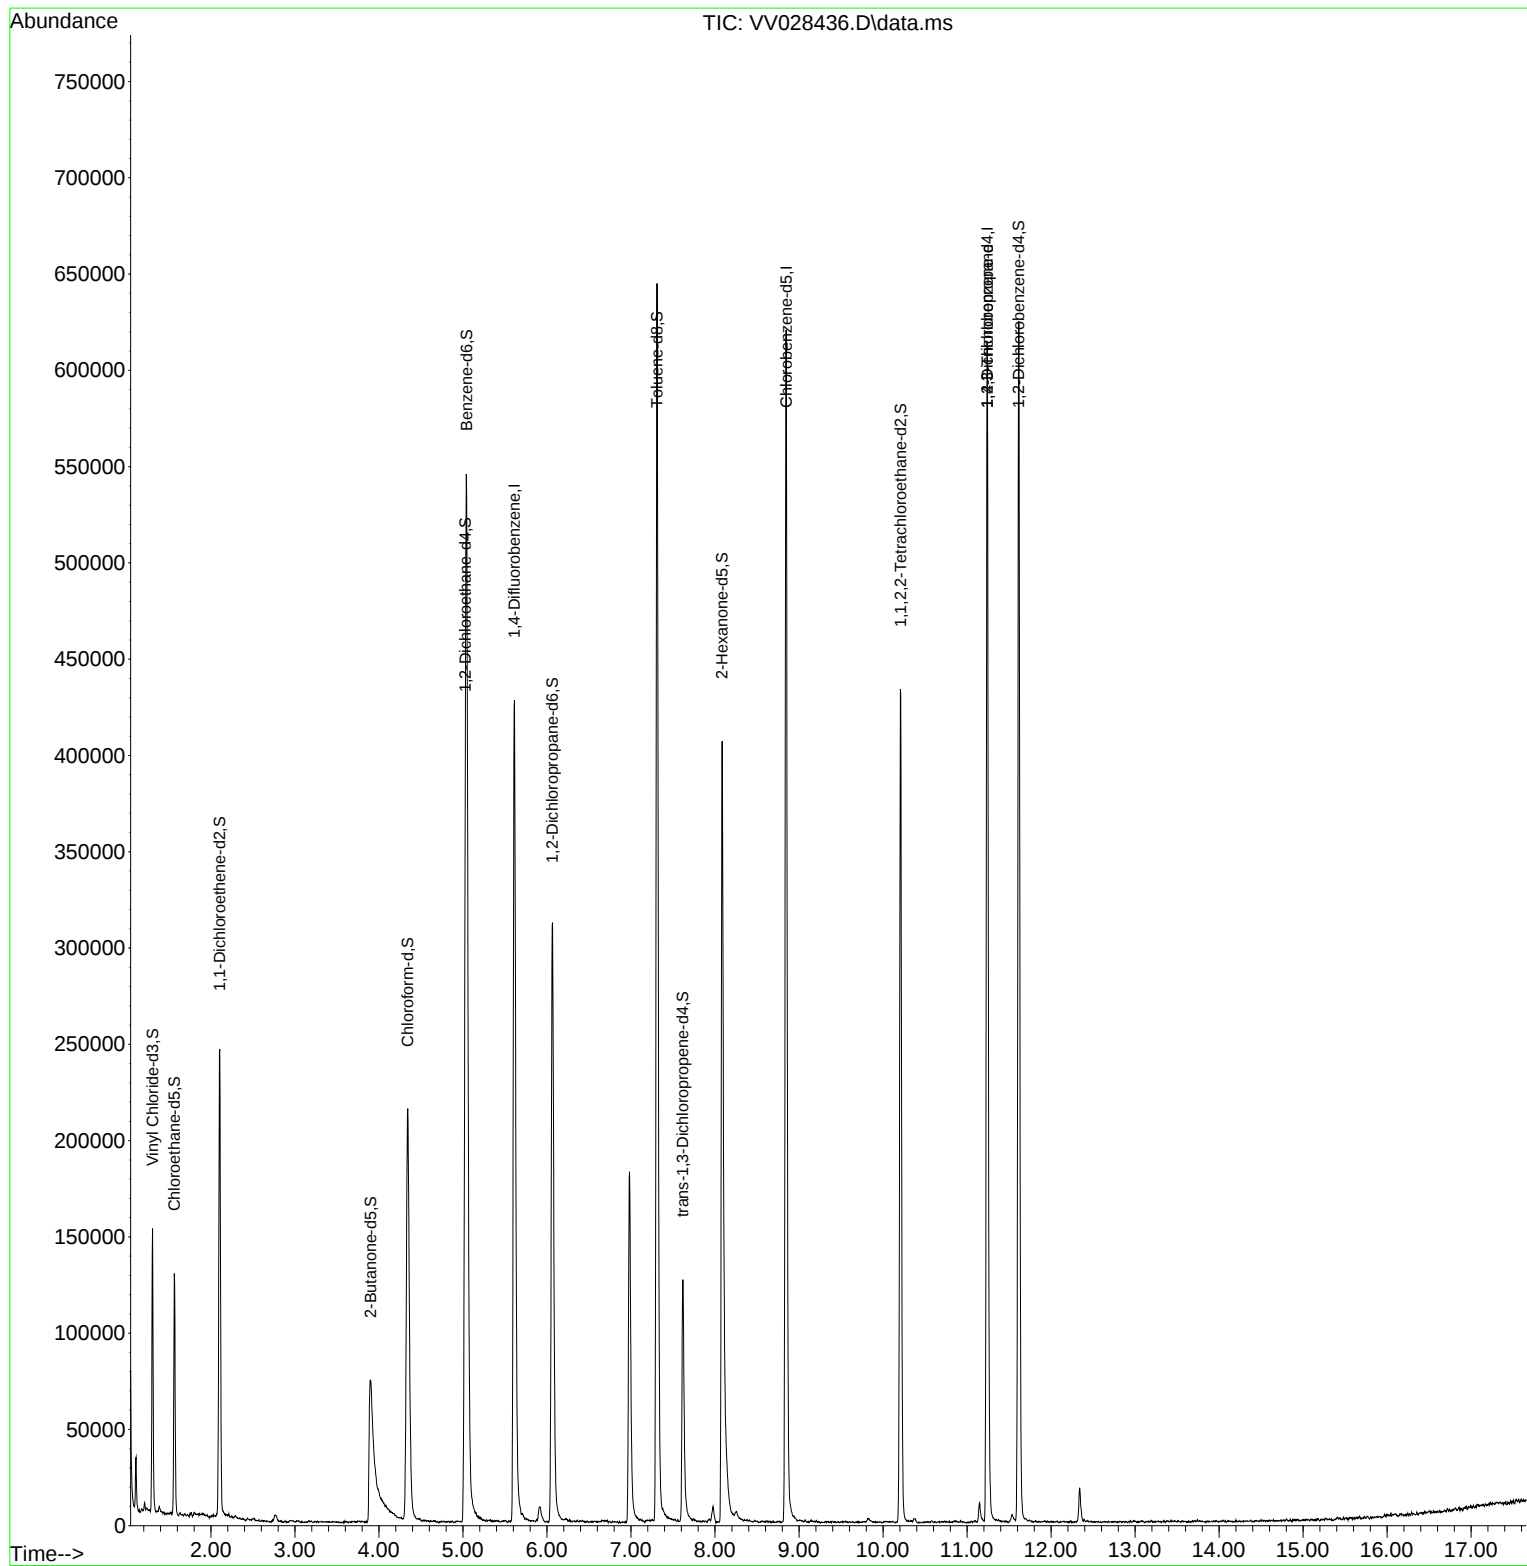

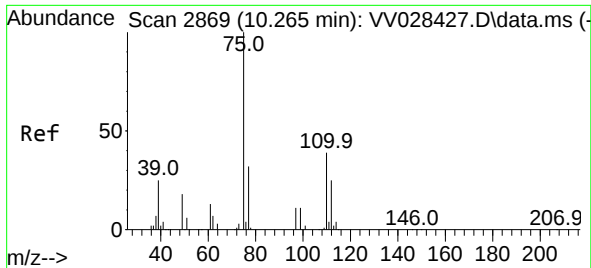

#61

1,2,3-Trichloropropane

Concen: 5.982 ug/L

RT: 11.239 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV028436.D


Acq: 08 Oct 2022 03:13

Instrument :

MSVOA_V

ClientSampleId :

BGSH2

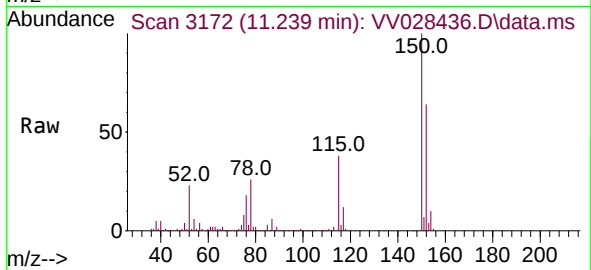

Tgt Ion: 75 Resp: 20282

Ion Ratio Lower Upper

75 100

77 33.0 25.7 38.5

110 2.7 30.0 45.0#

