




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

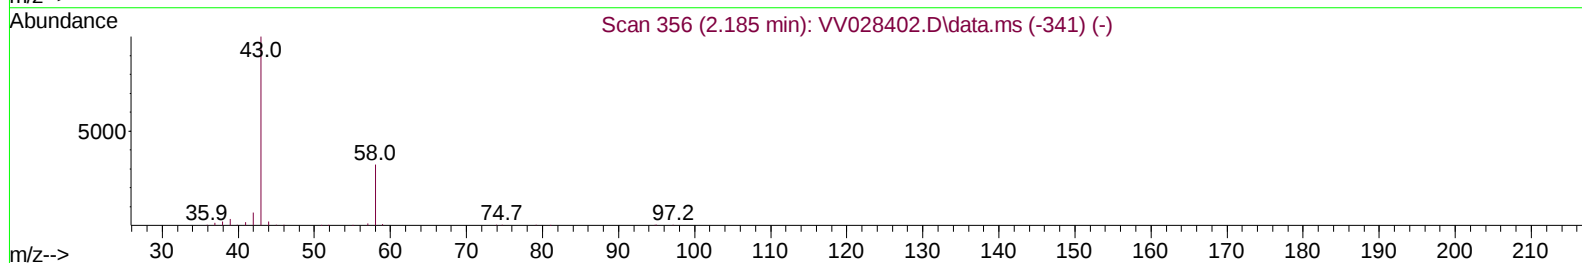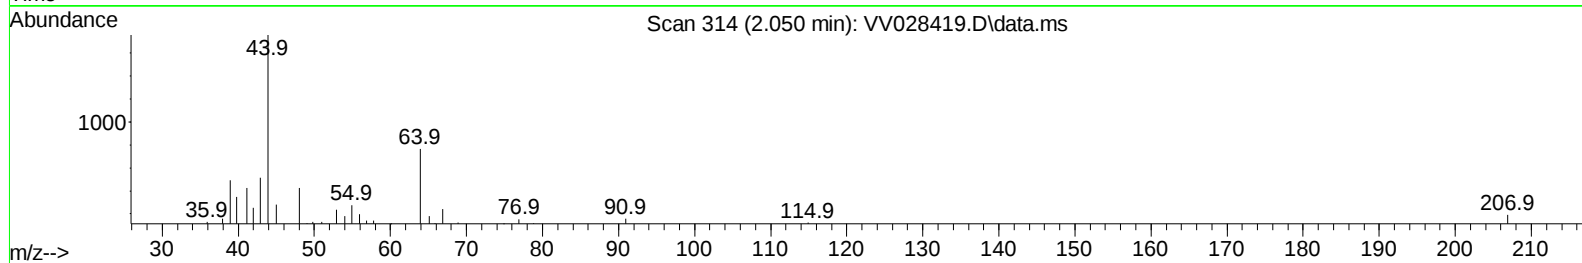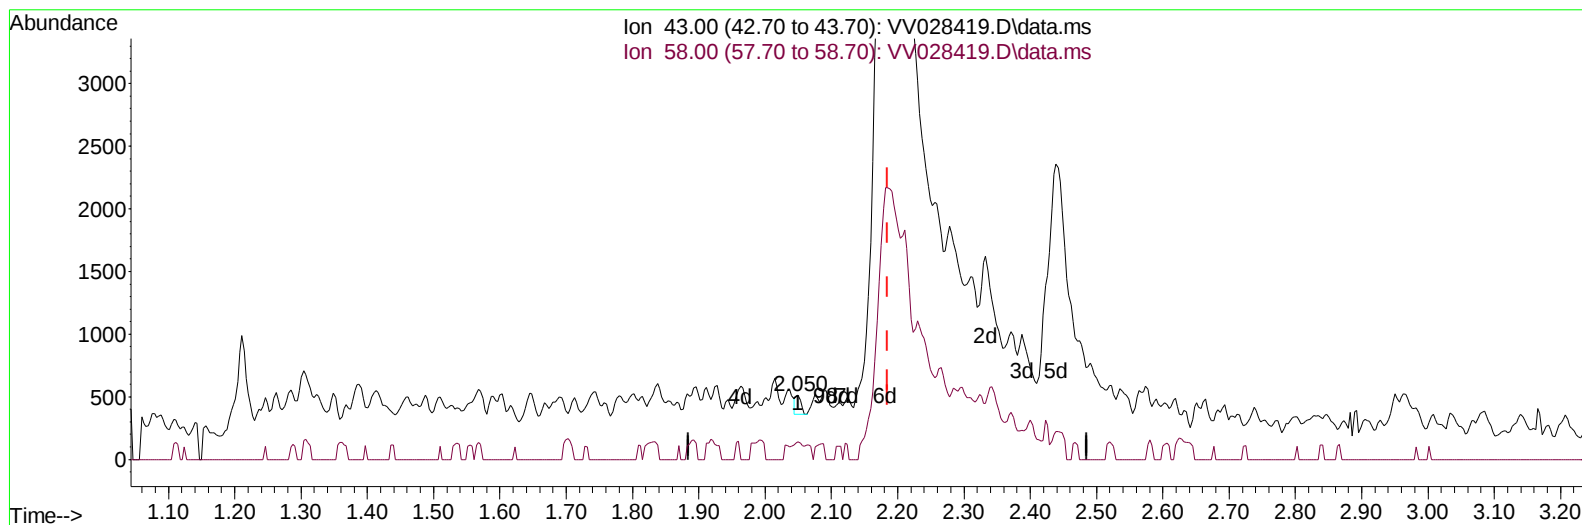

TIC: VV028419.D\data.ms

(13) Acetone (T)

2.050min (-0.135) 0.04 ug/L

response	91	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	23.50	19.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

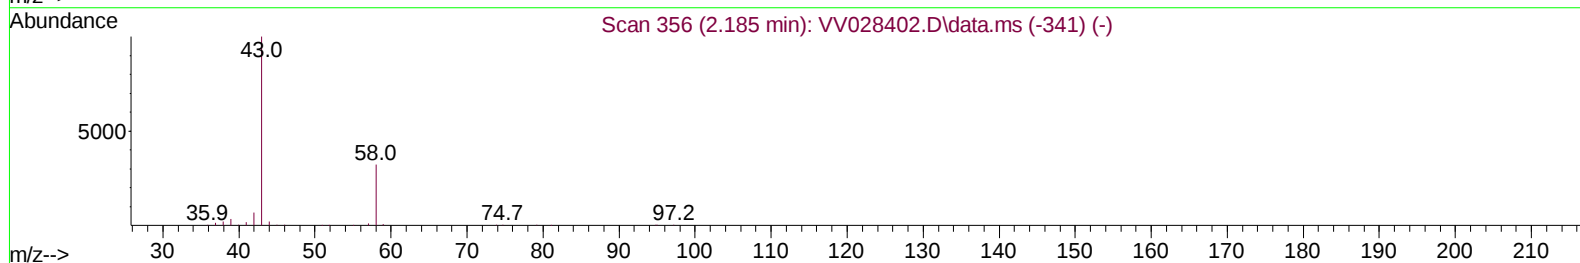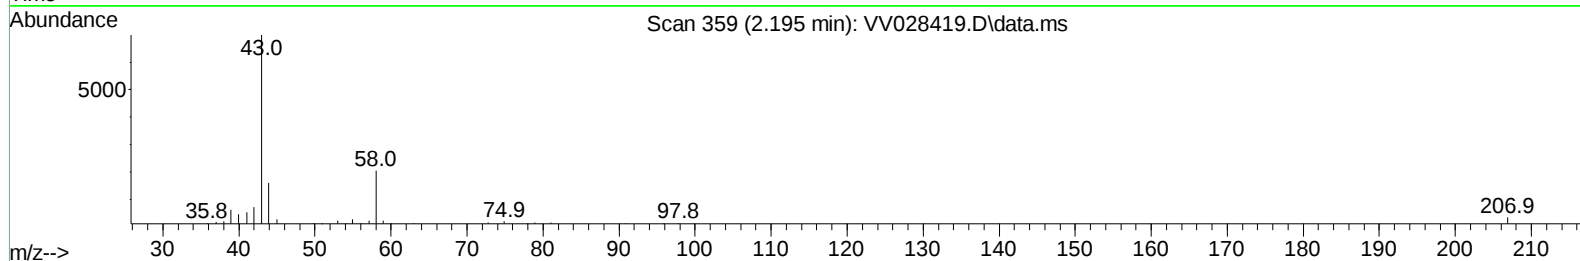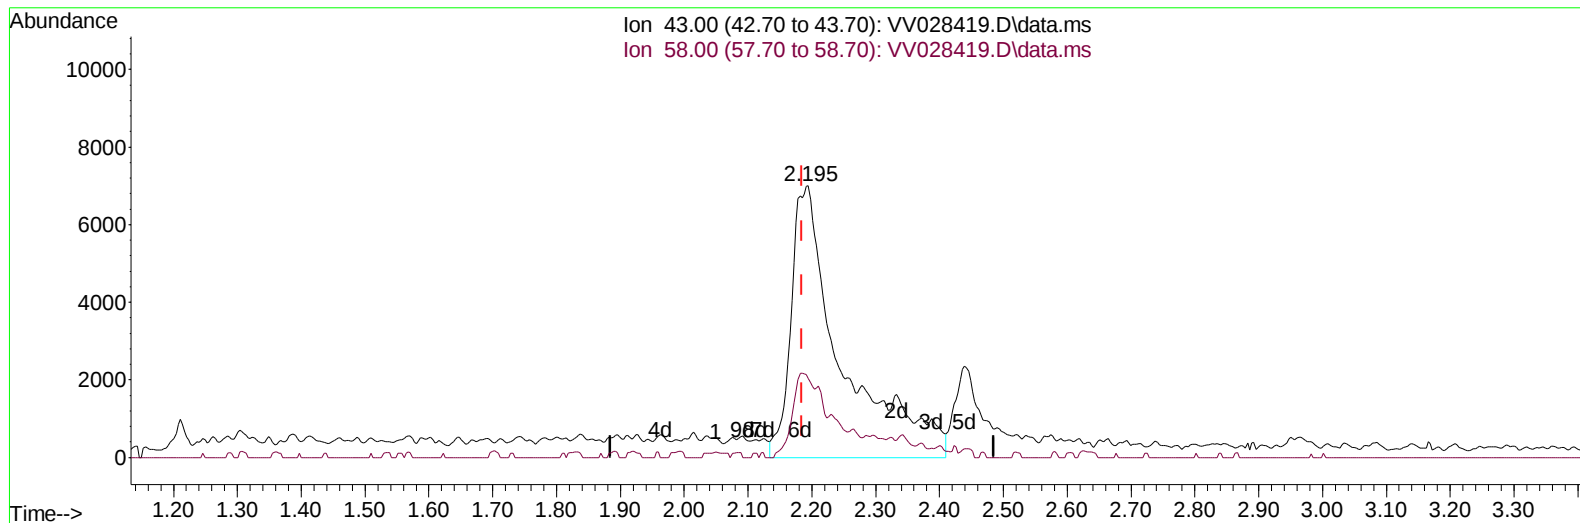

TIC: VV028419.D\data.ms

(13) Acetone (T)

2.195min (+ 0.009) 18.40 ug/L m

response 38441

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	23.50	0.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		399287	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117		361065	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152		171507	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		117453	38.123	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	76.240%	
7) Chloroethane-d5	1.564	69		98066	40.143	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	80.280%	
11) 1,1-Dichloroethene-d2	2.101	63		160220	30.556	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	61.120%	
21) 2-Butanone-d5	3.895	46		202510	75.086	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	75.090%	
24) Chloroform-d	4.342	84		257750	45.615	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.240%	
26) 1,2-Dichloroethane-d4	5.024	65		177456	48.696	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	97.400%	
32) Benzene-d6	5.043	84		542561	46.895	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	93.780%	
36) 1,2-Dichloropropane-d6	6.063	67		179134	47.488	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	94.980%	
41) Toluene-d8	7.310	98		488474	47.157	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	94.320%	
43) trans-1,3-Dichloroprop...	7.619	79		87671	45.597	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	91.200%	
47) 2-Hexanone-d5	8.085	63		184564	89.943	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	89.940%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		237319	45.975	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	91.940%	
66) 1,2-Dichlorobenzene-d4	11.615	152		176910	49.781	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	99.560%	
Target Compounds							
13) Acetone	2.195	43		38441m	18.400	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028419.D
Acq On : 07 Oct 2022 20:00
Operator : SY/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J63

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 23:51:49 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/10/2022

