




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028420.D
 Acq On : 07 Oct 2022 20:24
 Operator : SY/MD
 Sample : N4893-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J62

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

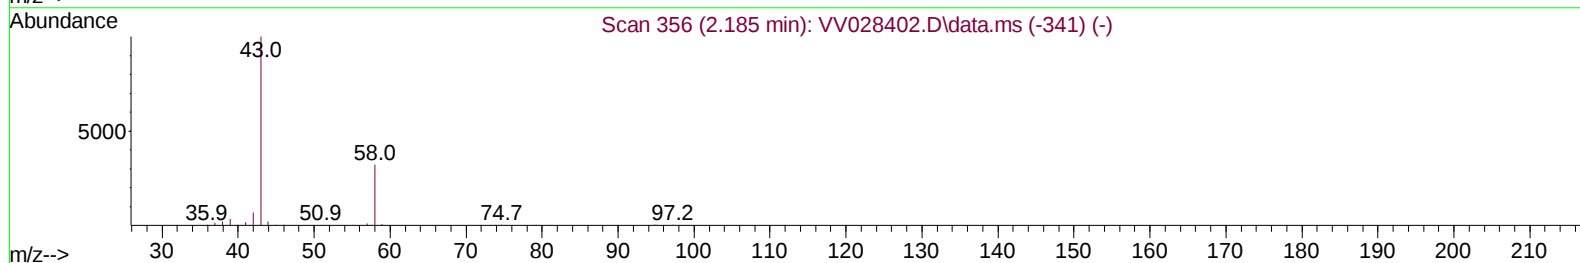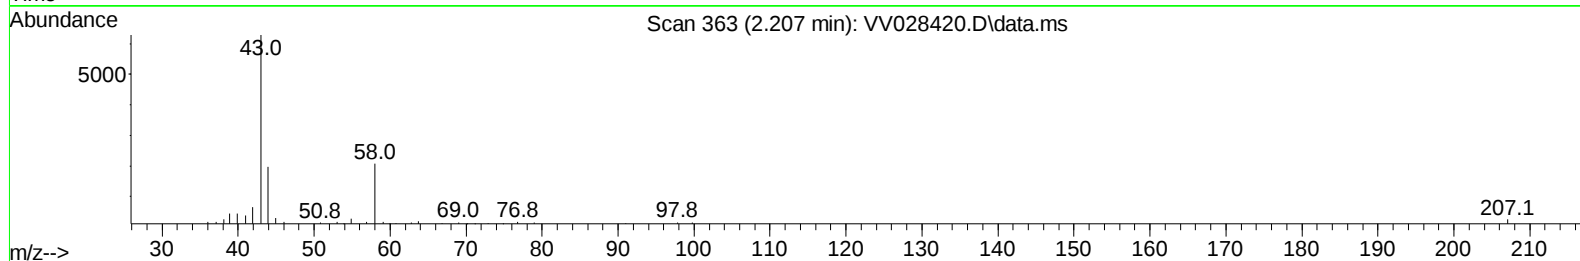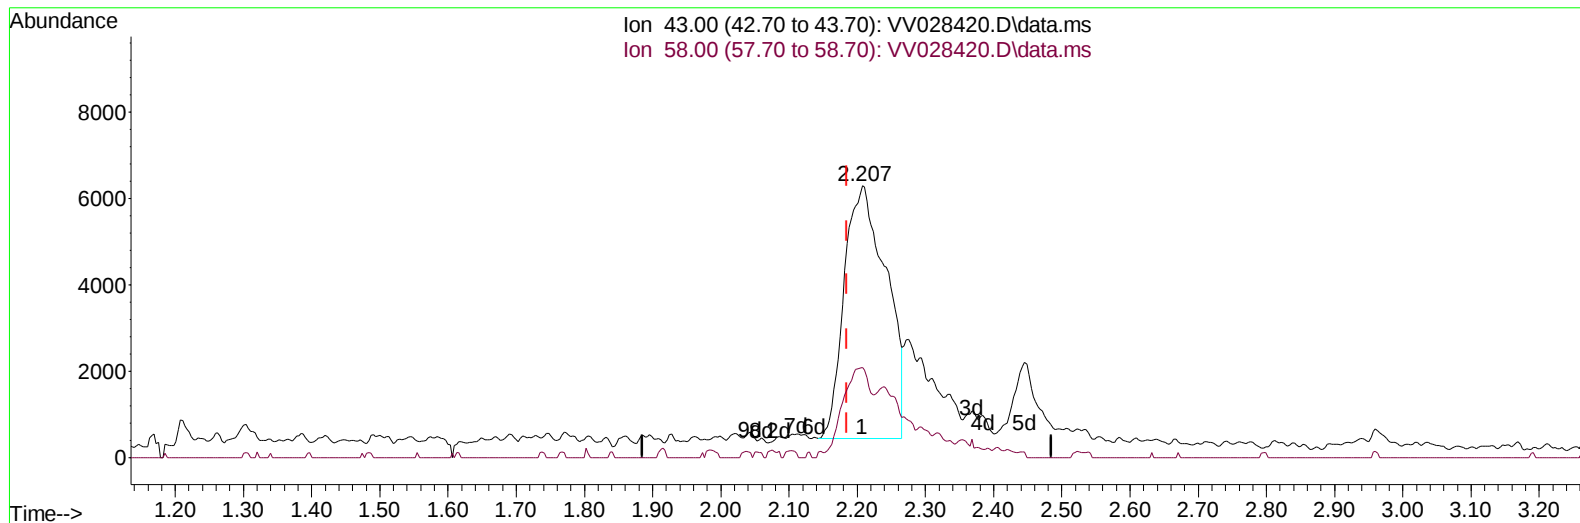

TIC: VV028420.D\data.ms

(13) Acetone (T)

2.207min (+ 0.022) 12.36 ug/L

response 25020

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	23.50	21.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028420.D
 Acq On : 07 Oct 2022 20:24
 Operator : SY/MD
 Sample : N4893-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J62

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

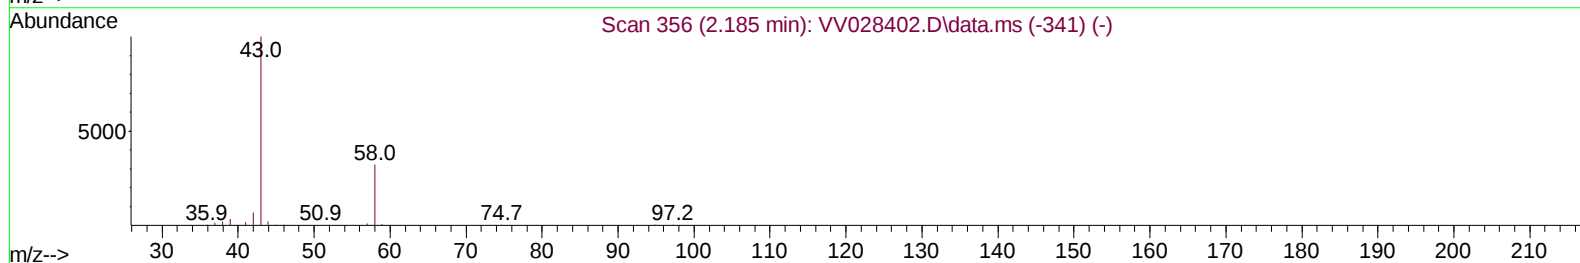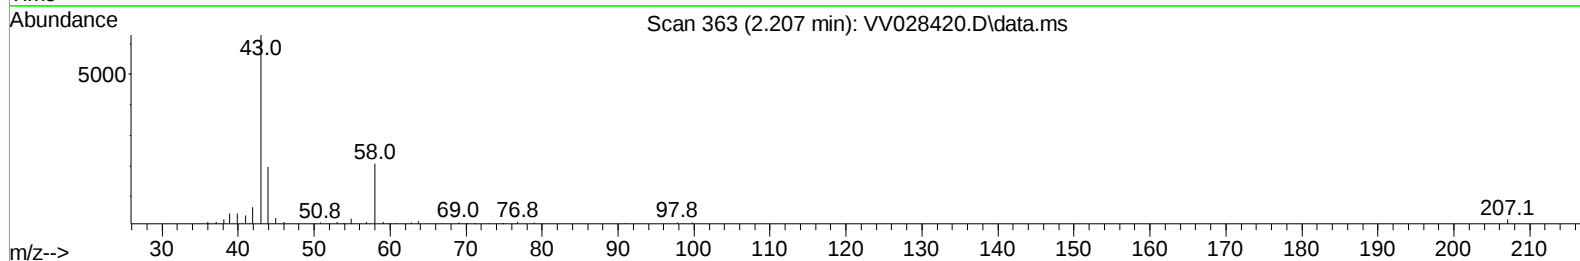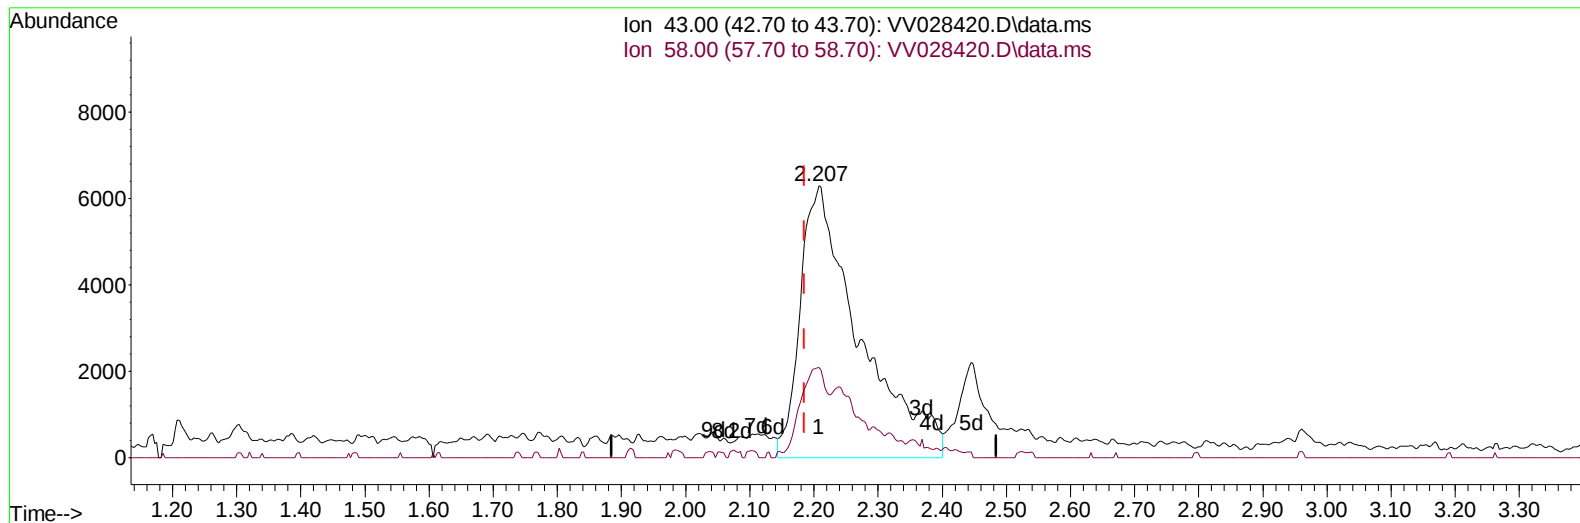

TIC: VV028420.D\data.ms

(13) Acetone (T)

2.207min (+ 0.022) 19.88 ug/L m

response 40248

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	23.50	13.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028420.D
 Acq On : 07 Oct 2022 20:24
 Operator : SY/MD
 Sample : N4893-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J62

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		386979	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117		345389	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152		166094	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		113468	38.001	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	76.000%	
7) Chloroethane-d5	1.564	69		97917	41.357	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	82.720%	
11) 1,1-Dichloroethene-d2	2.105	63		155949	30.687	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	61.380%	
21) 2-Butanone-d5	3.905	46		248178	94.945	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130		Recovery	=	94.950%	
24) Chloroform-d	4.342	84		250987	45.831	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.660%	
26) 1,2-Dichloroethane-d4	5.027	65		173792	49.207	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	98.420%	
32) Benzene-d6	5.043	84		527964	47.704	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.066	67		173236	48.009	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	96.020%	
41) Toluene-d8	7.310	98		473923	47.828	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	95.660%	
43) trans-1,3-Dichloroprop...	7.616	79		85972	46.743	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	93.480%	
47) 2-Hexanone-d5	8.085	63		186381	94.951	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	94.950%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		231235	46.829	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	93.660%	
66) 1,2-Dichlorobenzene-d4	11.615	152		170390	49.509	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	99.020%	
Target Compounds							
13) Acetone	2.207	43		40248m	19.877	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028420.D
Acq On : 07 Oct 2022 20:24
Operator : SY/MD
Sample : N4893-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
F5J62

Manual IntegrationsAPPROVED

Quant Time: Oct 08 01:02:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 23:51:49 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/10/2022

