

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028423.D
 Acq On : 07 Oct 2022 21:36
 Operator : SY/MD
 Sample : N4889-02 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ60

Quant Time: Oct 08 01:02:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 23:51:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	391331	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	351756	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	170271	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	104945	34.755	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.520%		
7) Chloroethane-d5	1.565	69	94599	39.511	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.020%		
11) 1,1-Dichloroethene-d2	2.101	63	150504	29.286	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	58.580%#		
21) 2-Butanone-d5	3.902	46	250142	94.632	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.630%		
24) Chloroform-d	4.343	84	246774	44.561	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.120%		
26) 1,2-Dichloroethane-d4	5.027	65	170434	47.720	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.440%		
32) Benzene-d6	5.043	84	519187	46.062	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.120%		
36) 1,2-Dichloropropane-d6	6.066	67	172456	46.927	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.860%		
41) Toluene-d8	7.310	98	468947	46.470	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.940%		
43) trans-1,3-Dichloroprop...	7.616	79	84908	45.329	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.660%		
47) 2-Hexanone-d5	8.085	63	185953	93.018	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.020%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	230848	45.905	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.800%		
66) 1,2-Dichlorobenzene-d4	11.616	152	170281	48.264	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.520%		
Target Compounds						Qvalue
35) Methylcyclohexane	6.130	83	4911	0.984	ug/L	96
42) Toluene	7.384	91	118592	9.945	ug/L	98
52) Ethylbenzene	9.008	91	191394	14.726	ug/L	99
53) m,p-Xylene	9.130	106	134839	27.371	ug/L	99
60) Isopropylbenzene	9.928	105	16553	1.349	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028423.D
Acq On : 07 Oct 2022 21:36
Operator : SY/MD
Sample : N4889-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ60

Quant Time: Oct 08 01:02:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 23:51:49 2022
Response via : Initial Calibration




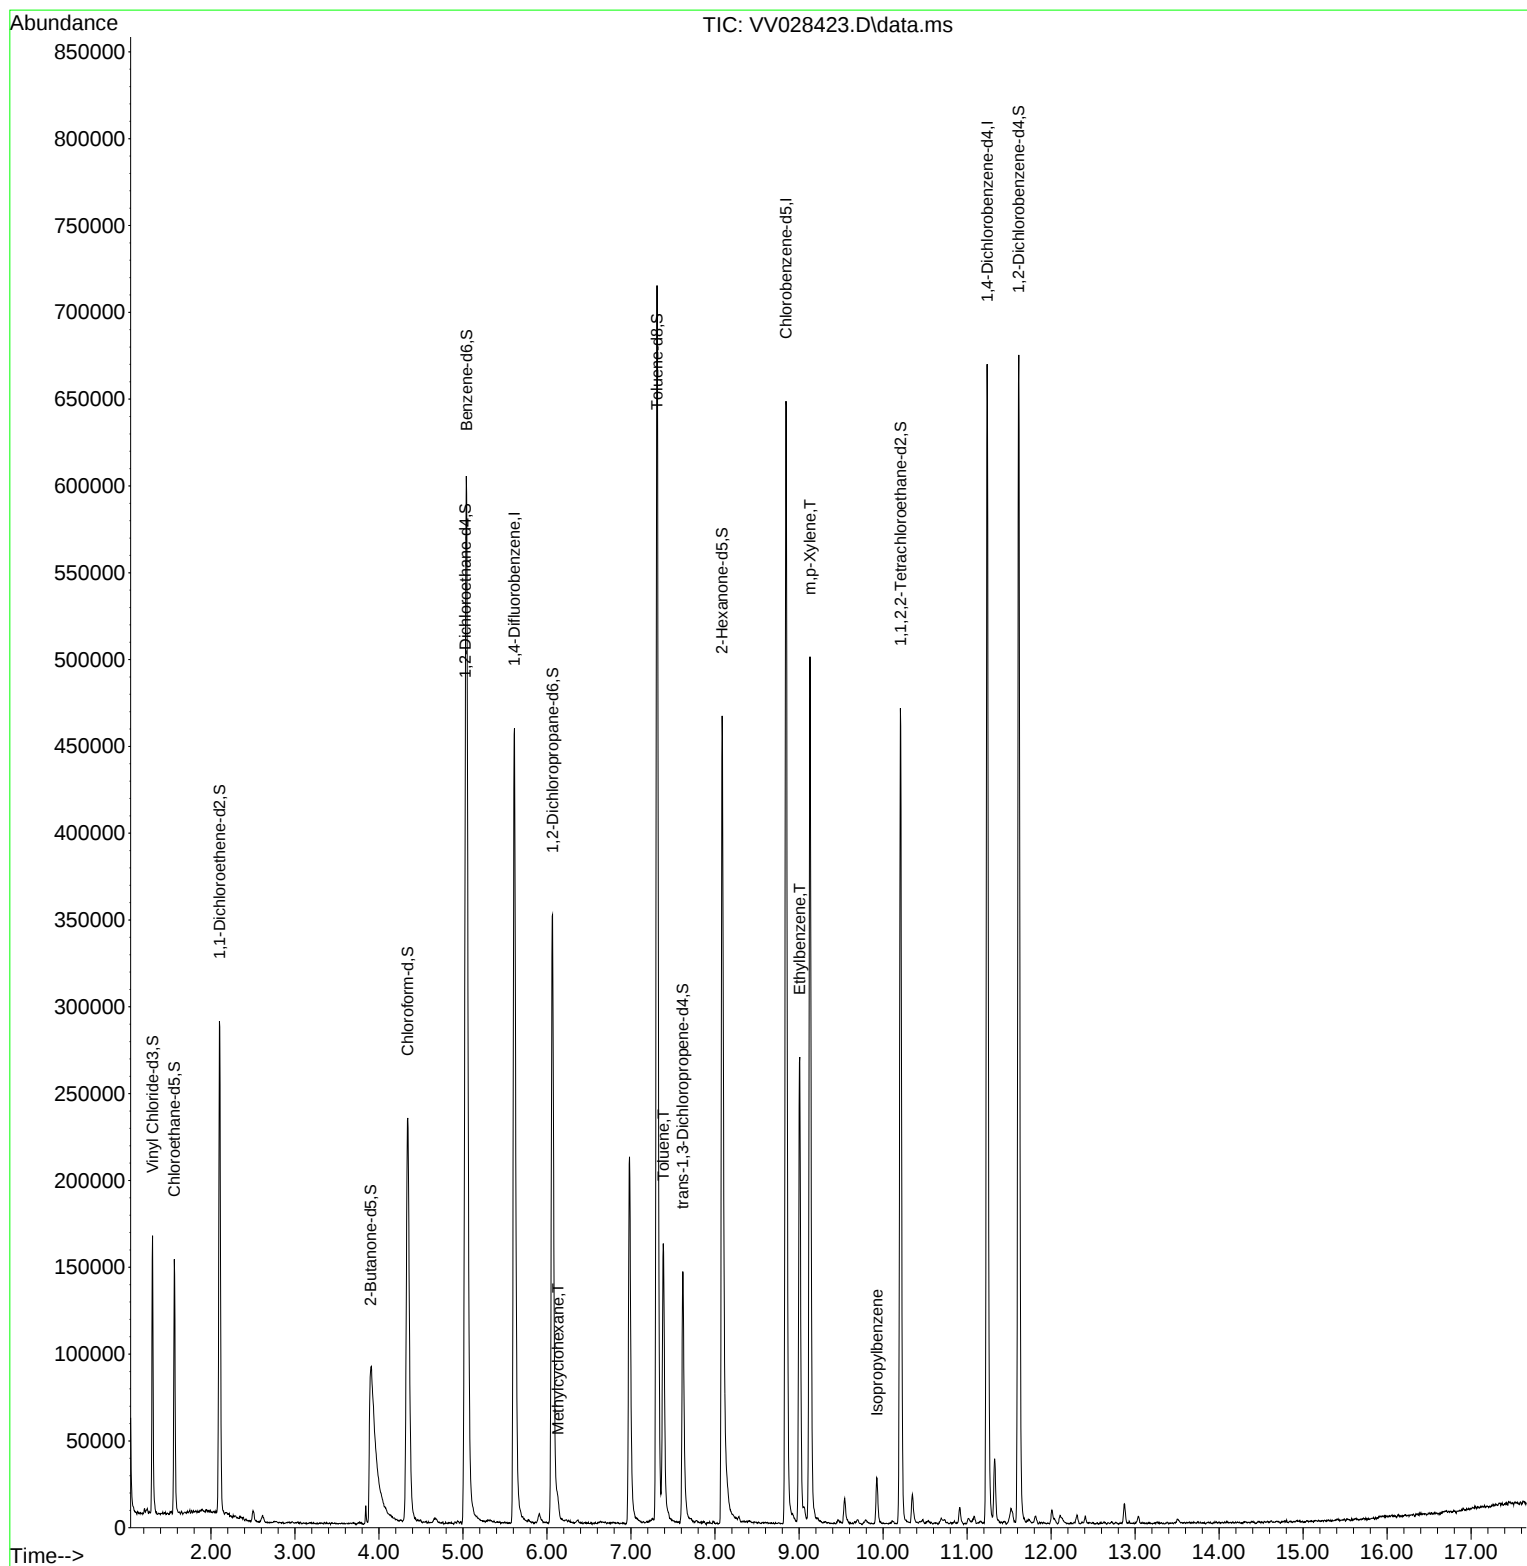


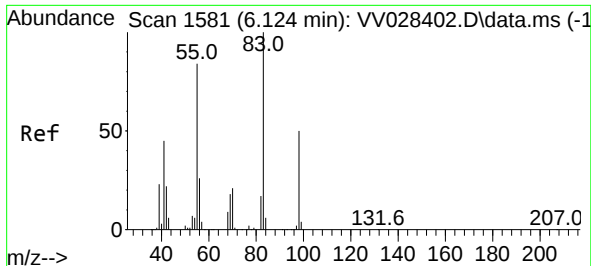

#35
Methylcyclohexane
Concen: 0.984 ug/L
RT: 6.130 min Scan# 11
Delta R.T. 0.006 min
Lab File: VV028423.D
Acq: 07 Oct 2022 21:36




Instrument :
MSVOA_V
ClientSampleId :
EXZ60


Tgt Ion: 83 Resp: 4911
Ion Ratio Lower Upper
83 100
55 79.5 63.7 95.5
98 40.4 38.2 57.2

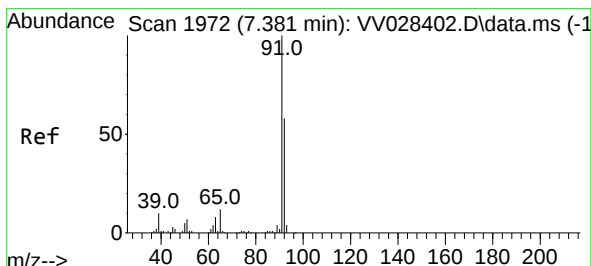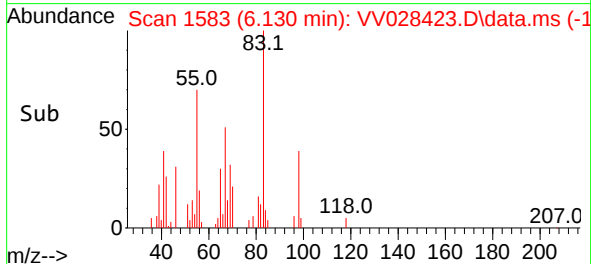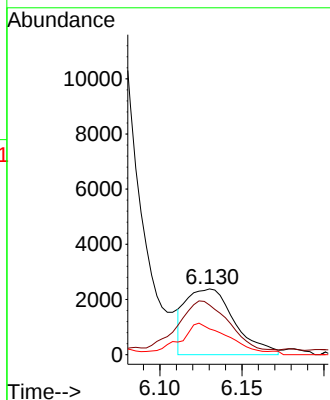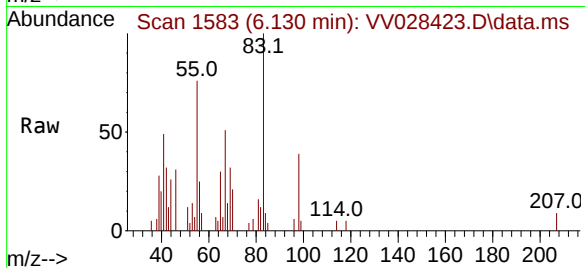

#42
Toluene
Concen: 9.945 ug/L
RT: 7.384 min Scan# 1973
Delta R.T. 0.003 min
Lab File: VV028423.D
Acq: 07 Oct 2022 21:36

Tgt Ion: 91 Resp: 118592
Ion Ratio Lower Upper
91 100
92 59.8 40.9 76.0


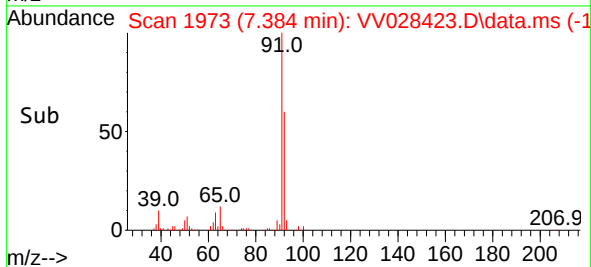
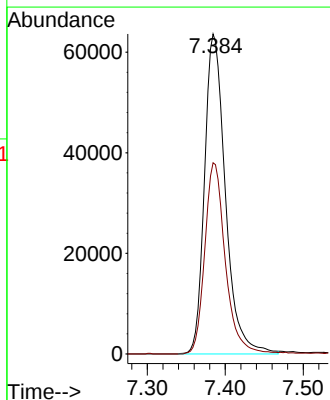
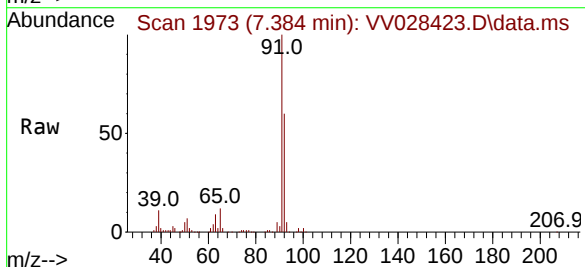


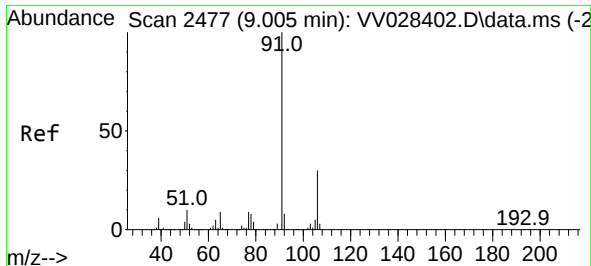

#52
Ethylbenzene
Concen: 14.726 ug/L
RT: 9.008 min Scan# 2477
Delta R.T. 0.003 min
Lab File: VV028423.D
Acq: 07 Oct 2022 21:36




Instrument :
MSVOA_V
ClientSampleId :
EXZ60


Tgt Ion: 91 Resp: 191394
Ion Ratio Lower Upper
91 100
106 30.2 21.4 39.8

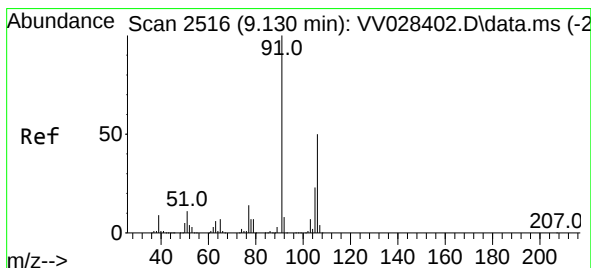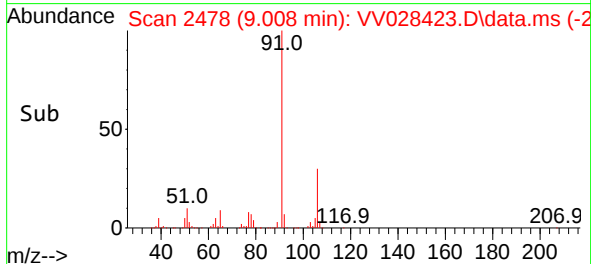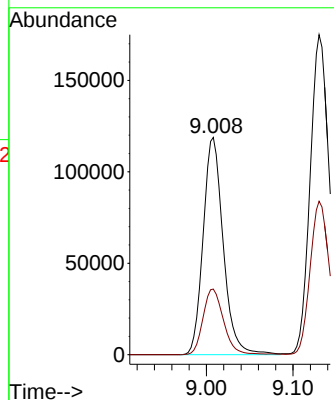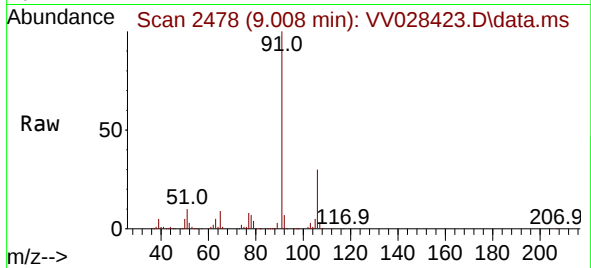

#53
m,p-Xylene
Concen: 27.371 ug/L
RT: 9.130 min Scan# 2516
Delta R.T. -0.000 min
Lab File: VV028423.D
Acq: 07 Oct 2022 21:36

Tgt Ion: 106 Resp: 134839
Ion Ratio Lower Upper
106 100
91 208.5 145.2 269.6

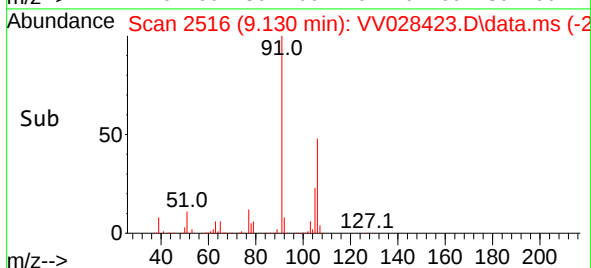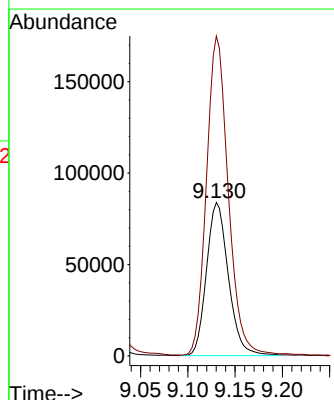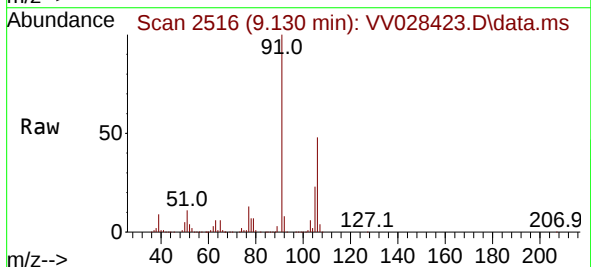

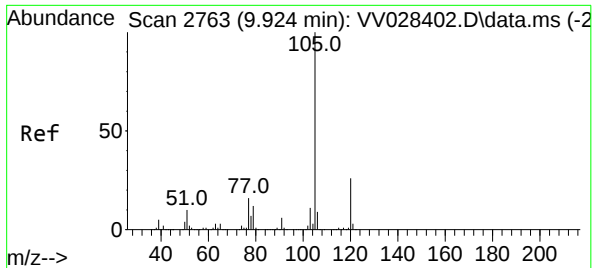

#60
Isopropylbenzene
Concen: 1.349 ug/L
RT: 9.928 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV028423.D
Acq: 07 Oct 2022 21:36

Instrument :
MSVOA_V
ClientSampleId :
EXZ60

Tgt Ion:	105	Resp:	16553
Ion	Ratio	Lower	Upper
105	100		
120	26.9	20.5	30.7
77	18.7	12.7	19.1

