

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028403.D
 Acq On : 07 Oct 2022 13:29
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	236954	251240	13.08%	1.731%
2	1.564	157	163	175	rVB	203222	229900	11.97%	1.584%
3	2.101	323	330	351	rVB	394243	575071	29.93%	3.961%
4	2.812	549	551	553	rBV3	953	299	0.02%	0.002%
5	3.056	625	627	632	rVB5	1035	516	0.03%	0.004%
6	3.082	632	635	636	rBV3	975	584	0.03%	0.004%
7	3.121	644	647	648	rBV2	1056	580	0.03%	0.004%
8	3.320	707	709	710	rBV2	667	282	0.01%	0.002%
9	3.365	722	723	727	rBV3	661	350	0.02%	0.002%
10	3.384	727	729	731	rBV2	577	286	0.01%	0.002%
11	3.564	779	785	788	rBV7	706	846	0.04%	0.006%
12	3.664	811	816	817	rBV6	1059	649	0.03%	0.004%
13	3.725	833	835	838	rBV4	735	414	0.02%	0.003%
14	3.764	842	847	848	rBV4	1024	706	0.04%	0.005%
15	3.773	848	850	854	rVB4	683	326	0.02%	0.002%
16	3.796	855	857	860	rBV4	589	307	0.02%	0.002%
17	3.902	879	890	928	rBV	102267	471326	24.53%	3.246%
18	4.342	1014	1027	1056	rVB	282466	711672	37.04%	4.902%
19	4.593	1103	1105	1106	rBV	1101	503	0.03%	0.003%
20	4.754	1153	1155	1158	rBV2	1072	846	0.04%	0.006%
21	4.950	1214	1216	1220	rVB5	1169	647	0.03%	0.004%
22	4.973	1220	1223	1224	rBV3	764	515	0.03%	0.004%
23	5.040	1227	1244	1272	rBV2	747000	1921109	100.00%	13.232%
24	5.613	1410	1422	1444	rBV	542161	1094983	57.00%	7.542%
25	6.066	1550	1563	1593	rBV	429975	885170	46.08%	6.097%
26	6.423	1671	1674	1680	rBV5	1328	1376	0.07%	0.009%
27	6.503	1695	1699	1704	rBV7	1163	1272	0.07%	0.009%
28	6.841	1802	1804	1807	rVB3	854	287	0.01%	0.002%
29	6.982	1836	1848	1879	rBV	265514	500961	26.08%	3.451%
30	7.310	1938	1950	1974	rBV	886680	1544671	80.41%	10.640%
31	7.616	2036	2045	2067	rBV	181512	321058	16.71%	2.211%
32	7.956	2148	2151	2152	rBV2	1278	645	0.03%	0.004%
33	8.021	2169	2171	2172	rBV2	972	305	0.02%	0.002%
34	8.047	2176	2179	2181	rBV3	810	537	0.03%	0.004%
35	8.085	2181	2191	2230	rBV	582114	1150802	59.90%	7.927%
36	8.542	2331	2333	2335	rBV3	785	444	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028403.D
 Acq On : 07 Oct 2022 13:29
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.751	2395	2398	2402	rBV5	933	632	0.03%	0.004%
38	8.844	2415	2427	2454	rBV	773785	1286505	66.97%	8.861%
39	9.243	2548	2551	2553	rBV3	636	380	0.02%	0.003%
40	9.268	2557	2559	2561	rBV3	915	411	0.02%	0.003%
41	9.310	2569	2572	2576	rBV5	1233	1225	0.06%	0.008%
42	9.497	2628	2630	2632	rBV2	441	225	0.01%	0.002%
43	9.506	2632	2633	2635	rBV2	631	250	0.01%	0.002%
44	9.625	2668	2670	2674	rVB4	1463	681	0.04%	0.005%
45	9.770	2711	2715	2716	rBV4	688	538	0.03%	0.004%
46	9.786	2718	2720	2722	rVV2	707	297	0.02%	0.002%
47	10.082	2810	2812	2814	rBV3	533	235	0.01%	0.002%
48	10.130	2825	2827	2829	rBV2	763	455	0.02%	0.003%
49	10.207	2839	2851	2870	rBV	578598	920793	47.93%	6.342%
50	10.474	2929	2934	2937	rBV5	855	924	0.05%	0.006%
51	10.532	2943	2952	2953	rBV6	2857	3424	0.18%	0.024%
52	10.699	3003	3004	3011	rVB6	935	489	0.03%	0.003%
53	10.751	3018	3020	3024	rBV4	728	452	0.02%	0.003%
54	10.808	3035	3038	3041	rVB4	743	361	0.02%	0.002%
55	10.825	3041	3043	3045	rBV3	1072	624	0.03%	0.004%
56	10.886	3060	3062	3064	rBV2	400	209	0.01%	0.001%
57	10.915	3064	3071	3076	rVV8	3394	4406	0.23%	0.030%
58	10.982	3089	3092	3095	rBV4	927	501	0.03%	0.003%
59	11.011	3097	3101	3105	rVB6	980	1024	0.05%	0.007%
60	11.062	3112	3117	3119	rBV5	931	847	0.04%	0.006%
61	11.091	3123	3126	3127	rBV3	714	422	0.02%	0.003%
62	11.107	3127	3131	3135	rVV6	671	658	0.03%	0.005%
63	11.149	3142	3144	3147	rVB4	986	581	0.03%	0.004%
64	11.178	3147	3153	3155	rBV5	4216	4402	0.23%	0.030%
65	11.239	3161	3172	3199	rBV	796315	1246472	64.88%	8.586%
66	11.413	3224	3226	3230	rBV3	950	745	0.04%	0.005%
67	11.516	3256	3258	3260	rBV3	893	357	0.02%	0.002%
68	11.545	3263	3267	3269	rVB4	1241	870	0.05%	0.006%
69	11.558	3269	3271	3272	rBV2	639	224	0.01%	0.002%
70	11.615	3277	3289	3310	rBV	820482	1307803	68.08%	9.008%
71	11.853	3361	3363	3364	rBV2	861	372	0.02%	0.003%
72	12.001	3407	3409	3410	rBV2	629	225	0.01%	0.002%
73	12.014	3410	3413	3415	rVV4	957	505	0.03%	0.003%
74	12.027	3415	3417	3423	rVB6	1317	1107	0.06%	0.008%
75	12.088	3433	3436	3437	rBV2	1009	508	0.03%	0.003%
76	12.210	3470	3474	3476	rBV5	1164	823	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028403.D
 Acq On : 07 Oct 2022 13:29
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.230	3478	3480	3484	rVB5	1313	831	0.04%	0.006%
78	12.249	3484	3486	3488	rBV3	411	216	0.01%	0.001%
79	12.400	3528	3533	3536	rBV6	1258	1231	0.06%	0.008%
80	12.416	3536	3538	3539	rBV2	830	407	0.02%	0.003%
81	12.493	3561	3562	3563	rBV	714	271	0.01%	0.002%
82	12.558	3579	3582	3584	rBV3	964	613	0.03%	0.004%
83	12.590	3590	3592	3596	rBV3	1080	600	0.03%	0.004%
84	12.644	3602	3609	3620	rVB3	5277	10336	0.54%	0.071%
85	12.689	3620	3623	3626	rBV4	2181	1602	0.08%	0.011%
86	12.763	3644	3646	3647	rBV2	945	410	0.02%	0.003%
87	12.792	3653	3655	3657	rBV2	647	387	0.02%	0.003%
88	12.831	3664	3667	3669	rBV4	1083	703	0.04%	0.005%
89	12.921	3691	3695	3701	rBV7	923	941	0.05%	0.006%
90	13.165	3768	3771	3773	rBV4	768	403	0.02%	0.003%
91	13.255	3793	3799	3811	rVB6	6357	10761	0.56%	0.074%
92	13.451	3858	3860	3862	rBV3	819	415	0.02%	0.003%
93	13.503	3868	3876	3888	rBV2	11523	20197	1.05%	0.139%
94	13.590	3900	3903	3904	rBV3	1082	565	0.03%	0.004%
95	13.644	3917	3920	3921	rBV2	848	425	0.02%	0.003%
96	13.702	3935	3938	3939	rBV3	785	429	0.02%	0.003%
97	13.860	3985	3987	3991	rBV5	1366	925	0.05%	0.006%
98	13.969	4018	4021	4023	rBV4	1301	784	0.04%	0.005%
99	14.445	4167	4169	4172	rBV5	1410	698	0.04%	0.005%
100	14.651	4231	4233	4235	rBV3	1169	515	0.03%	0.004%




Sum of corrected areas: 14518112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028403.D
Acq On : 07 Oct 2022 13:29
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

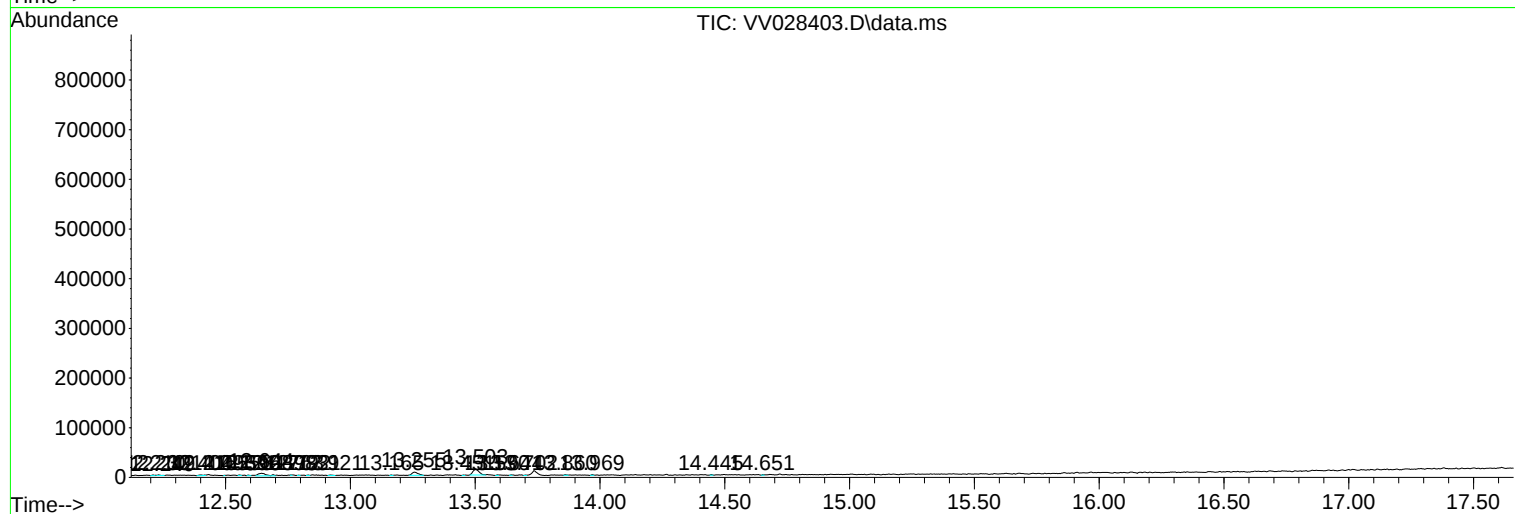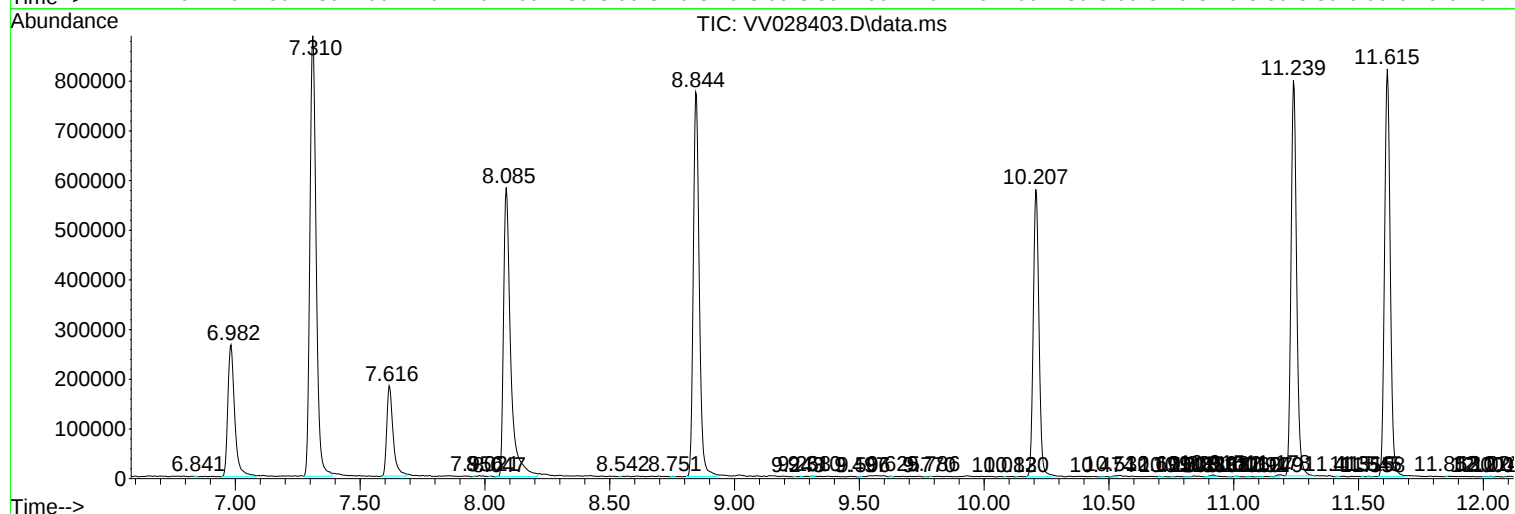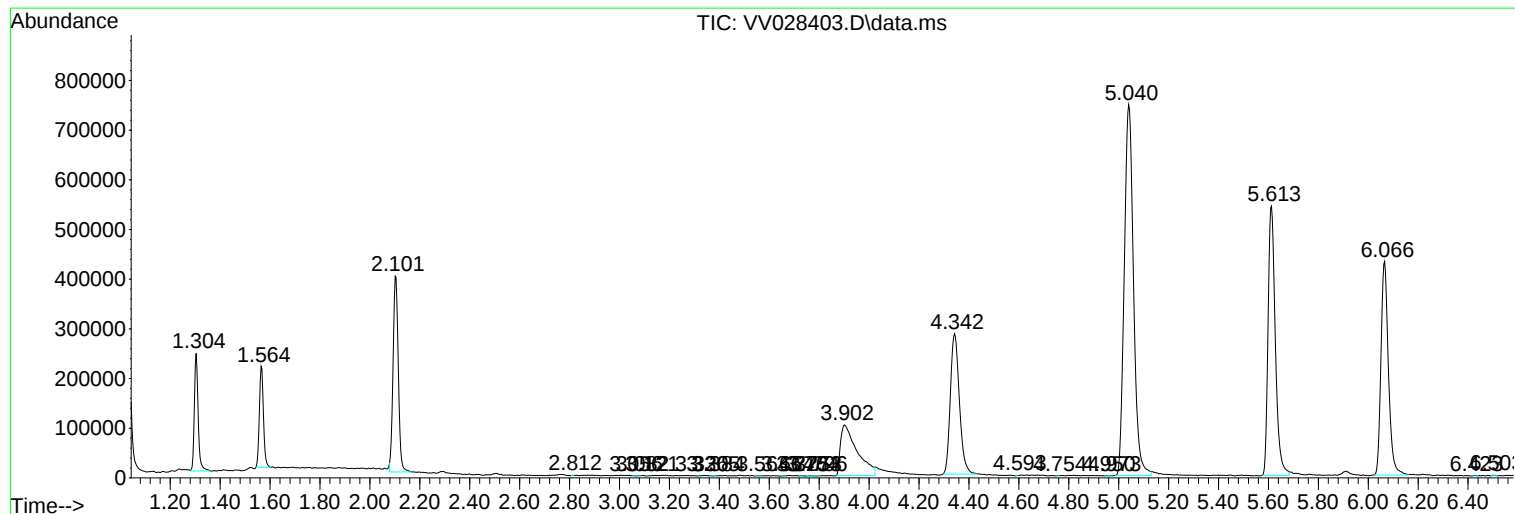

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028403.D
Acq On : 07 Oct 2022 13:29
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028403.D
Acq On : 07 Oct 2022 13:29
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------