

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028408.D
 Acq On : 07 Oct 2022 15:36
 Operator : SY/MD
 Sample : N4853-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	221970	224208	12.27%	1.634%
2	1.564	157	163	175	rVB	189439	212854	11.65%	1.552%
3	2.105	322	331	345	rVB	368675	526112	28.80%	3.835%
4	2.706	516	518	520	rBV3	1235	620	0.03%	0.005%
5	3.143	652	654	656	rBV3	936	372	0.02%	0.003%
6	3.159	656	659	662	rBV4	1072	785	0.04%	0.006%
7	3.317	706	708	709	rBV2	831	352	0.02%	0.003%
8	3.343	714	716	720	rBV5	964	742	0.04%	0.005%
9	3.404	733	735	741	rBV4	711	542	0.03%	0.004%
10	3.587	790	792	793	rBV2	824	385	0.02%	0.003%
11	3.613	797	800	801	rBV2	1068	605	0.03%	0.004%
12	3.687	820	823	828	rBV6	1150	852	0.05%	0.006%
13	3.744	839	841	845	rVB4	1278	753	0.04%	0.005%
14	3.818	860	864	867	rBV4	702	627	0.03%	0.005%
15	3.834	867	869	870	rBV2	724	345	0.02%	0.003%
16	3.892	876	887	920	rBV3	120372	479769	26.27%	3.497%
17	4.343	1012	1027	1056	rBV	273216	691302	37.85%	5.039%
18	4.770	1158	1160	1164	rBV4	1045	598	0.03%	0.004%
19	4.892	1196	1198	1200	rBV3	794	327	0.02%	0.002%
20	4.931	1206	1210	1211	rBV3	1085	744	0.04%	0.005%
21	4.966	1218	1221	1226	rBV6	891	630	0.03%	0.005%
22	5.040	1226	1244	1272	rBV2	708888	1826560	100.00%	13.315%
23	5.613	1410	1422	1452	rBV	509414	1045628	57.25%	7.622%
24	6.063	1548	1562	1586	rBV	405016	840794	46.03%	6.129%
25	6.452	1680	1683	1685	rBV3	862	445	0.02%	0.003%
26	6.471	1685	1689	1692	rBV5	795	752	0.04%	0.005%
27	6.619	1732	1735	1737	rBV3	803	360	0.02%	0.003%
28	6.815	1793	1796	1798	rBV4	1699	1167	0.06%	0.009%
29	6.934	1830	1833	1834	rBV3	662	321	0.02%	0.002%
30	6.982	1834	1848	1874	rBV	243203	465470	25.48%	3.393%
31	7.310	1938	1950	1975	rBV	844864	1467130	80.32%	10.695%
32	7.567	2028	2030	2035	rBV6	1130	1000	0.05%	0.007%
33	7.616	2036	2045	2069	rBV2	168443	305620	16.73%	2.228%
34	8.040	2175	2177	2179	rBV3	639	322	0.02%	0.002%
35	8.085	2181	2191	2225	rVV	525668	1053832	57.69%	7.682%
36	8.606	2350	2353	2357	rBV6	868	691	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028408.D
 Acq On : 07 Oct 2022 15:36
 Operator : SY/MD
 Sample : N4853-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.693	2376	2380	2383	rVB5	1290	951	0.05%	0.007%
38	8.847	2416	2428	2454	rBV	745618	1227610	67.21%	8.949%
39	9.255	2553	2555	2557	rBV2	1018	623	0.03%	0.005%
40	9.326	2574	2577	2580	rBV4	731	579	0.03%	0.004%
41	9.352	2582	2585	2587	rBV3	840	519	0.03%	0.004%
42	9.387	2594	2596	2599	rBV3	649	370	0.02%	0.003%
43	9.403	2599	2601	2606	rVB5	1341	1046	0.06%	0.008%
44	9.426	2606	2608	2611	rBV3	1162	817	0.04%	0.006%
45	9.503	2629	2632	2634	rBV3	1241	687	0.04%	0.005%
46	9.516	2634	2636	2638	rVV3	1214	571	0.03%	0.004%
47	9.542	2642	2644	2651	rVV7	1078	1103	0.06%	0.008%
48	9.664	2679	2682	2684	rBV3	778	540	0.03%	0.004%
49	9.702	2693	2694	2695	rBV	892	217	0.01%	0.002%
50	9.735	2702	2704	2707	rVB4	810	320	0.02%	0.002%
51	9.770	2711	2715	2718	rBV4	971	956	0.05%	0.007%
52	9.821	2729	2731	2733	rBV2	848	551	0.03%	0.004%
53	10.072	2803	2809	2811	rBV5	800	746	0.04%	0.005%
54	10.207	2840	2851	2874	rBV	539935	865180	47.37%	6.307%
55	10.509	2940	2945	2946	rBV4	1069	847	0.05%	0.006%
56	10.651	2986	2989	2991	rBV4	853	488	0.03%	0.004%
57	10.706	3004	3006	3009	rBV4	934	520	0.03%	0.004%
58	10.738	3014	3016	3017	rBV	719	285	0.02%	0.002%
59	10.783	3028	3030	3031	rBV2	726	265	0.01%	0.002%
60	10.892	3060	3064	3065	rBV3	762	501	0.03%	0.004%
61	10.998	3095	3097	3100	rBV4	903	688	0.04%	0.005%
62	11.120	3132	3135	3137	rBV3	986	767	0.04%	0.006%
63	11.156	3144	3146	3147	rBV2	564	220	0.01%	0.002%
64	11.239	3161	3172	3197	rBV	750491	1190476	65.18%	8.678%
65	11.616	3277	3289	3314	rBV	786313	1251794	68.53%	9.125%
66	11.857	3362	3364	3365	rBV2	594	214	0.01%	0.002%
67	11.870	3366	3368	3370	rVV3	738	352	0.02%	0.003%
68	12.030	3415	3418	3421	rBV3	1075	575	0.03%	0.004%
69	12.053	3421	3425	3429	rVV5	1351	1127	0.06%	0.008%
70	12.210	3471	3474	3476	rBV4	1277	820	0.04%	0.006%
71	12.349	3513	3517	3519	rBV4	1213	996	0.05%	0.007%
72	12.484	3557	3559	3562	rVB2	1031	520	0.03%	0.004%
73	12.500	3562	3564	3566	rBV3	807	455	0.02%	0.003%
74	12.548	3576	3579	3580	rBV3	766	481	0.03%	0.004%
75	12.612	3596	3599	3601	rBV3	968	737	0.04%	0.005%
76	12.751	3640	3642	3643	rBV	691	335	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028408.D
 Acq On : 07 Oct 2022 15:36
 Operator : SY/MD
 Sample : N4853-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

77	12.918	3692	3694	3697	rVB5	1257	607	0.03%	0.004%
78	12.934	3697	3699	3701	rBV2	1073	558	0.03%	0.004%
79	13.024	3724	3727	3729	rBV4	782	477	0.03%	0.003%
80	13.313	3815	3817	3821	rBV4	670	481	0.03%	0.004%
81	13.345	3825	3827	3831	rBV4	922	604	0.03%	0.004%
82	13.397	3836	3843	3845	rVB7	1389	1347	0.07%	0.010%
83	13.609	3905	3909	3911	rBV3	962	651	0.04%	0.005%
84	13.648	3917	3921	3925	rBV5	967	877	0.05%	0.006%
85	13.705	3937	3939	3941	rBV3	1157	612	0.03%	0.004%
86	14.075	4052	4054	4057	rBV3	1200	485	0.03%	0.004%
87	14.297	4120	4123	4125	rBV4	1070	707	0.04%	0.005%




Sum of corrected areas: 13717871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028408.D
Acq On : 07 Oct 2022 15:36
Operator : SY/MD
Sample : N4853-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

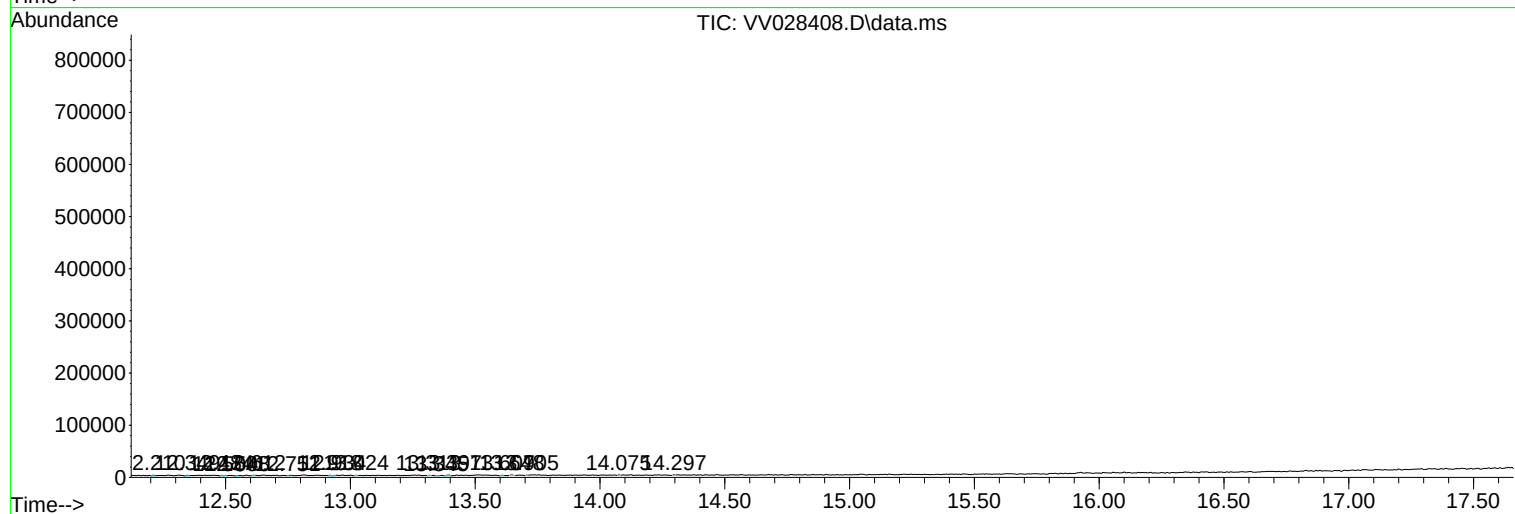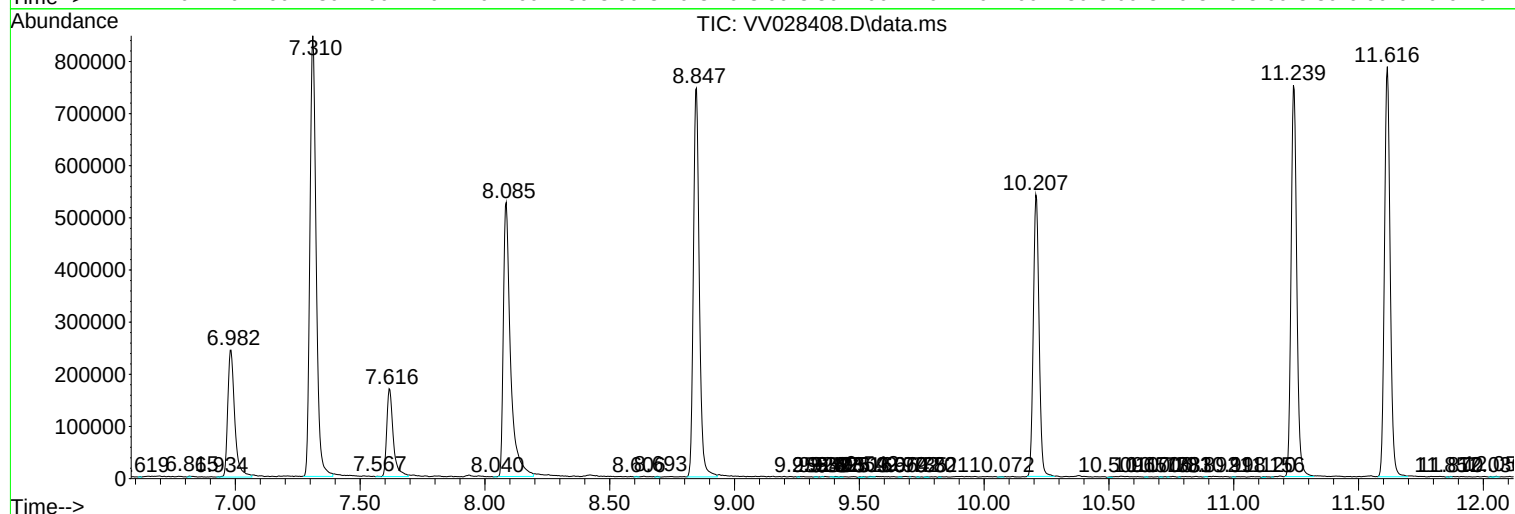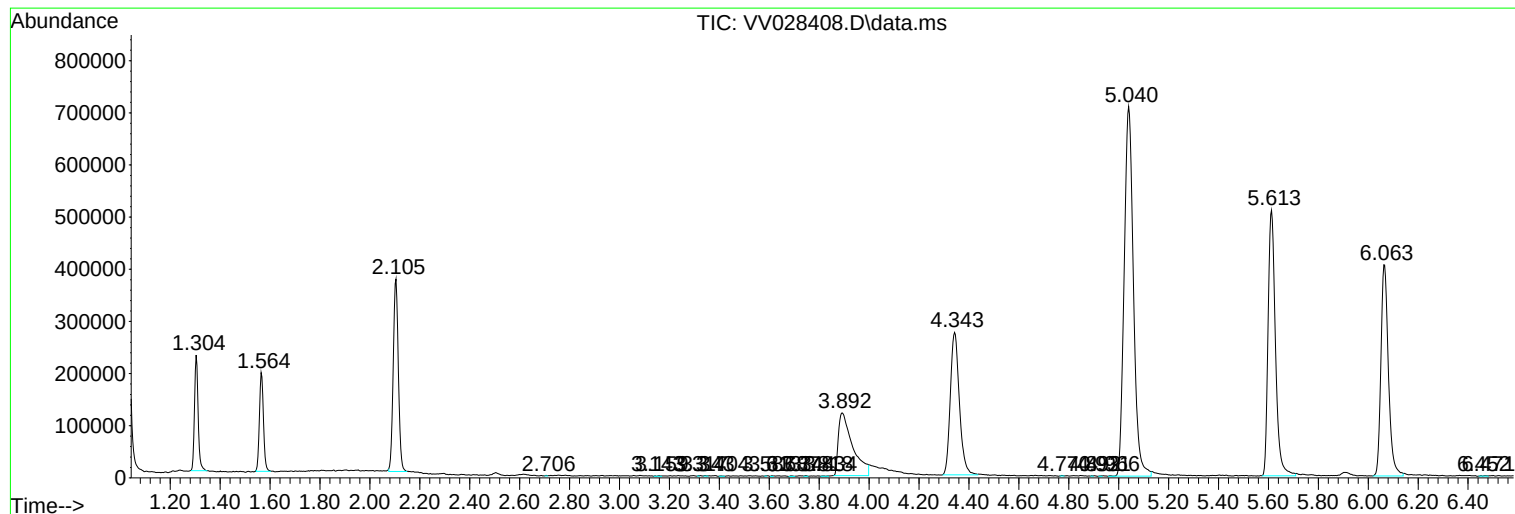

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028408.D
Acq On : 07 Oct 2022 15:36
Operator : SY/MD
Sample : N4853-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028408.D
Acq On : 07 Oct 2022 15:36
Operator : SY/MD
Sample : N4853-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------