

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028409.D
 Acq On : 07 Oct 2022 16:00
 Operator : SY/MD
 Sample : N4890-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	211292	217651	12.28%	1.616%
2	1.564	157	163	176	rVB	181653	206453	11.65%	1.533%
3	2.105	322	331	346	rVB	347233	504144	28.44%	3.743%
4	2.899	576	578	581	rVB3	1417	626	0.04%	0.005%
5	3.079	631	634	636	rBV3	898	554	0.03%	0.004%
6	3.098	636	640	642	rVV3	870	674	0.04%	0.005%
7	3.130	648	650	652	rBV3	493	262	0.01%	0.002%
8	3.191	667	669	672	rBV4	773	466	0.03%	0.003%
9	3.207	672	674	679	rVB4	1333	1056	0.06%	0.008%
10	3.236	679	683	688	rBV6	1523	1830	0.10%	0.014%
11	3.471	751	756	758	rBV6	948	766	0.04%	0.006%
12	3.526	770	773	775	rBV3	850	615	0.03%	0.005%
13	3.571	784	787	789	rBV3	1303	885	0.05%	0.007%
14	3.648	808	811	813	rBV2	994	711	0.04%	0.005%
15	3.677	818	820	822	rBV2	851	370	0.02%	0.003%
16	3.712	827	831	835	rBV5	798	561	0.03%	0.004%
17	3.783	851	853	857	rBV5	1080	666	0.04%	0.005%
18	3.899	876	889	936	rBV2	127116	581518	32.80%	4.318%
19	4.342	1013	1027	1063	rVB	266228	674293	38.04%	5.007%
20	4.651	1121	1123	1125	rBV3	958	454	0.03%	0.003%
21	4.770	1158	1160	1162	rBV2	924	562	0.03%	0.004%
22	4.822	1173	1176	1179	rBV4	1260	1097	0.06%	0.008%
23	4.867	1188	1190	1193	rBV3	677	383	0.02%	0.003%
24	4.931	1208	1210	1214	rBV6	785	345	0.02%	0.003%
25	5.040	1227	1244	1286	rBV2	690034	1772816	100.00%	13.164%
26	5.612	1409	1422	1448	rBV	493991	1019441	57.50%	7.570%
27	6.066	1548	1563	1585	rBV	394661	817031	46.09%	6.067%
28	6.513	1700	1702	1704	rBV3	796	392	0.02%	0.003%
29	6.638	1735	1741	1743	rBV7	975	1048	0.06%	0.008%
30	6.783	1785	1786	1789	rVB3	907	298	0.02%	0.002%
31	6.802	1789	1792	1798	rBV5	1054	1339	0.08%	0.010%
32	6.886	1815	1818	1820	rBV4	388	287	0.02%	0.002%
33	6.982	1837	1848	1881	rVV	241555	453488	25.58%	3.367%
34	7.310	1939	1950	1974	rBV	802912	1404847	79.24%	10.431%
35	7.616	2036	2045	2071	rBV	166819	299734	16.91%	2.226%
36	7.818	2106	2108	2112	rBV4	1303	977	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028409.D
 Acq On : 07 Oct 2022 16:00
 Operator : SY/MD
 Sample : N4890-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.889	2128	2130	2131	rBV2	1424	533	0.03%	0.004%
38	8.085	2181	2191	2237	rBV	553699	1069819	60.35%	7.944%
39	8.545	2332	2334	2337	rBV3	788	469	0.03%	0.003%
40	8.680	2372	2376	2381	rBV7	1226	1018	0.06%	0.008%
41	8.709	2381	2385	2386	rBV2	1062	668	0.04%	0.005%
42	8.783	2404	2408	2410	rBV5	741	599	0.03%	0.004%
43	8.844	2416	2427	2456	rBV	706466	1184274	66.80%	8.793%
44	9.130	2515	2516	2517	rBV	719	268	0.02%	0.002%
45	9.345	2580	2583	2586	rBV5	1022	602	0.03%	0.004%
46	9.387	2593	2596	2598	rBV4	935	505	0.03%	0.004%
47	9.426	2606	2608	2609	rBV2	787	416	0.02%	0.003%
48	9.464	2617	2620	2621	rBV3	621	341	0.02%	0.003%
49	9.538	2641	2643	2645	rVV2	754	449	0.03%	0.003%
50	9.567	2648	2652	2657	rBV7	1409	1259	0.07%	0.009%
51	9.632	2670	2672	2674	rVB3	808	313	0.02%	0.002%
52	9.648	2674	2677	2679	rBV4	1014	564	0.03%	0.004%
53	9.670	2682	2684	2689	rVB4	1034	737	0.04%	0.005%
54	9.715	2693	2698	2700	rBV5	983	900	0.05%	0.007%
55	9.744	2706	2707	2710	rVB2	896	360	0.02%	0.003%
56	9.760	2710	2712	2716	rBV4	729	471	0.03%	0.003%
57	9.831	2730	2734	2737	rBV4	684	404	0.02%	0.003%
58	9.934	2762	2766	2767	rBV4	1407	702	0.04%	0.005%
59	10.114	2819	2822	2827	rBV5	989	1015	0.06%	0.008%
60	10.207	2840	2851	2873	rVV	537025	850342	47.97%	6.314%
61	10.374	2894	2903	2907	rBV10	2383	3722	0.21%	0.028%
62	10.435	2917	2922	2923	rBV4	815	577	0.03%	0.004%
63	10.471	2930	2933	2937	rBV4	681	636	0.04%	0.005%
64	10.509	2943	2945	2948	rBV4	625	369	0.02%	0.003%
65	10.525	2948	2950	2953	rBV4	954	651	0.04%	0.005%
66	10.603	2971	2974	2979	rBV6	1198	1174	0.07%	0.009%
67	10.657	2988	2991	2992	rBV2	610	343	0.02%	0.003%
68	10.715	3006	3009	3010	rBV3	670	362	0.02%	0.003%
69	10.818	3037	3041	3045	rBV4	643	587	0.03%	0.004%
70	10.844	3047	3049	3052	rVV3	618	327	0.02%	0.002%
71	10.918	3066	3072	3073	rBV5	854	696	0.04%	0.005%
72	11.024	3103	3105	3106	rBV	628	262	0.01%	0.002%
73	11.140	3138	3141	3143	rBV4	643	459	0.03%	0.003%
74	11.178	3148	3153	3157	rBV6	1923	2097	0.12%	0.016%
75	11.239	3161	3172	3194	rBV	739393	1147788	64.74%	8.523%
76	11.503	3249	3254	3257	rBV5	724	738	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028409.D
 Acq On : 07 Oct 2022 16:00
 Operator : SY/MD
 Sample : N4890-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.522	3257	3260	3262	rBV5	546	367	0.02%	0.003%
78	11.615	3274	3289	3307	rBV	755602	1208074	68.14%	8.970%
79	11.808	3347	3349	3352	rBV4	1158	573	0.03%	0.004%
80	11.963	3395	3397	3401	rVB4	741	489	0.03%	0.004%
81	11.982	3401	3403	3405	rBV3	619	271	0.02%	0.002%
82	12.021	3413	3415	3418	rVB3	1039	462	0.03%	0.003%
83	12.168	3459	3461	3464	rVB4	700	327	0.02%	0.002%
84	12.191	3464	3468	3469	rBV4	1003	631	0.04%	0.005%
85	12.246	3483	3485	3489	rBV5	1111	872	0.05%	0.006%
86	12.358	3516	3520	3523	rBV6	685	593	0.03%	0.004%
87	12.461	3549	3552	3553	rBV3	619	351	0.02%	0.003%
88	12.503	3563	3565	3568	rBV5	551	299	0.02%	0.002%
89	12.599	3591	3595	3598	rBV5	1019	906	0.05%	0.007%
90	12.709	3627	3629	3632	rBV4	718	335	0.02%	0.002%
91	13.001	3718	3720	3725	rVV5	806	418	0.02%	0.003%
92	13.059	3735	3738	3741	rBV4	836	535	0.03%	0.004%
93	13.133	3758	3761	3763	rVB4	1246	630	0.04%	0.005%
94	13.146	3763	3765	3768	rBV3	807	438	0.02%	0.003%
95	13.268	3801	3803	3805	rBV3	982	588	0.03%	0.004%
96	13.439	3854	3856	3858	rVB3	882	339	0.02%	0.003%
97	13.471	3861	3866	3867	rBV4	1267	984	0.06%	0.007%
98	13.574	3896	3898	3903	rVB6	815	527	0.03%	0.004%
99	13.609	3905	3909	3913	rBV6	1255	1324	0.07%	0.010%
100	13.869	3987	3990	3992	rBV3	1207	846	0.05%	0.006%




Sum of corrected areas: 13467635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028409.D
Acq On : 07 Oct 2022 16:00
Operator : SY/MD
Sample : N4890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

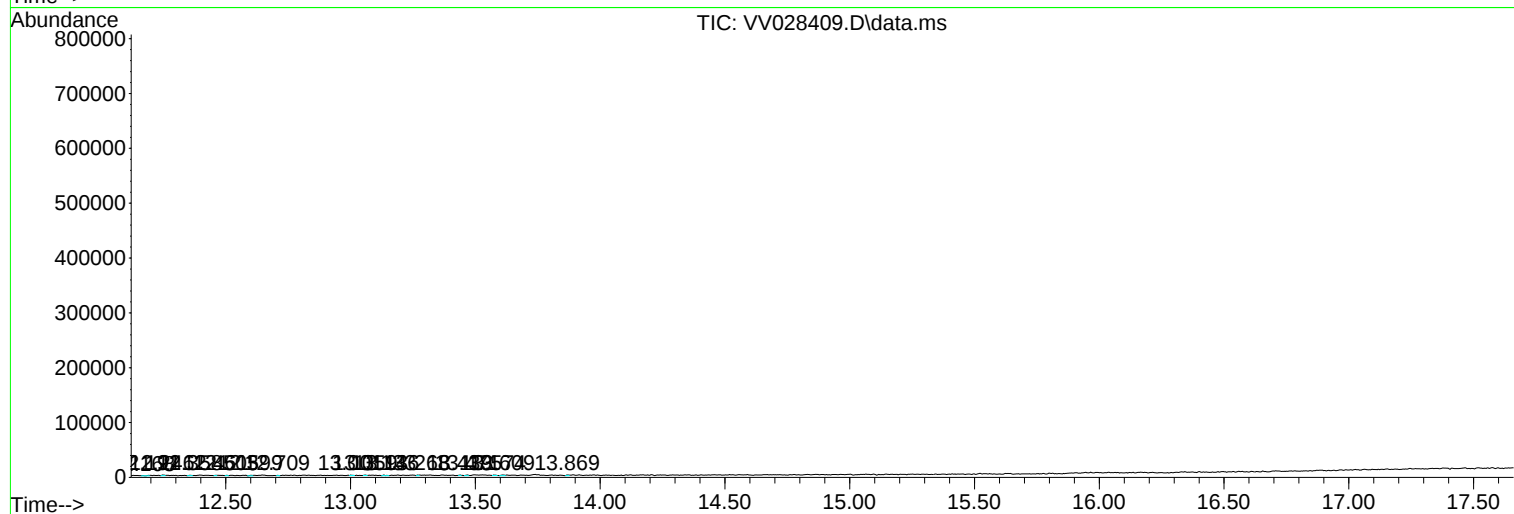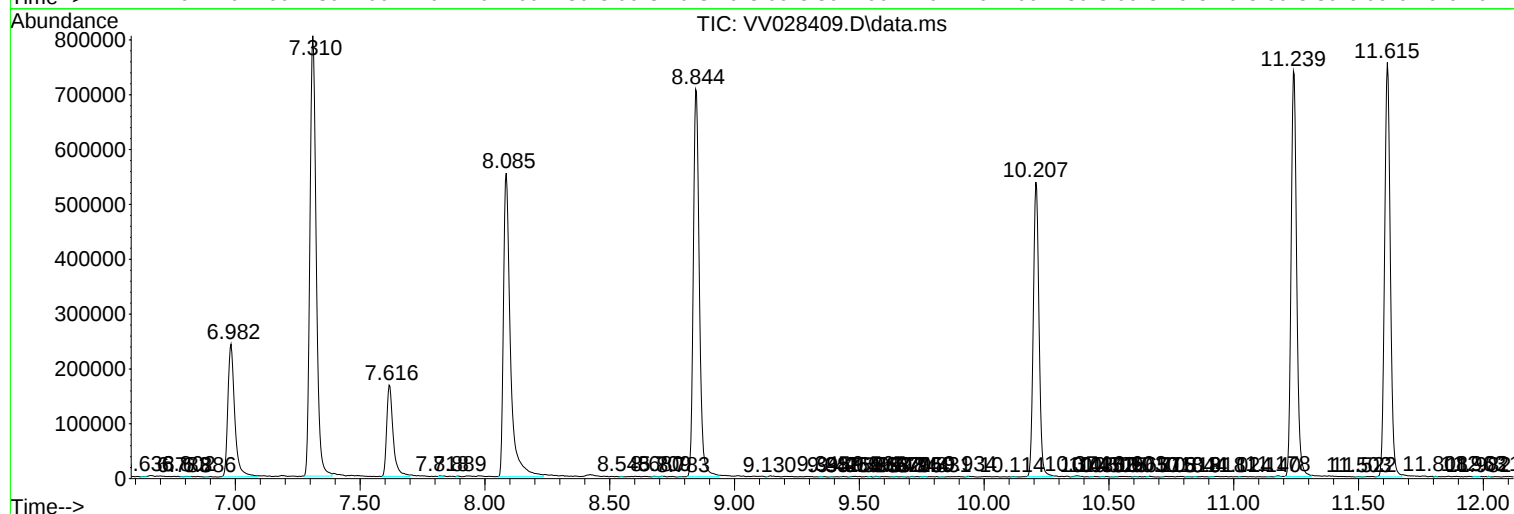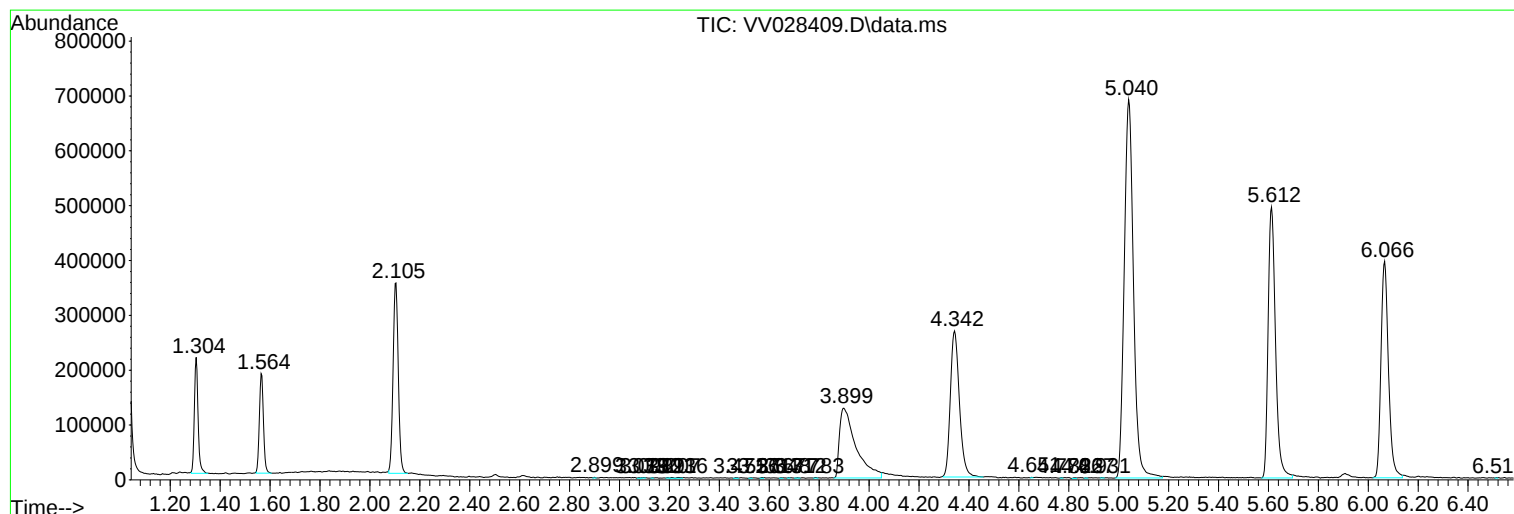

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028409.D
Acq On : 07 Oct 2022 16:00
Operator : SY/MD
Sample : N4890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028409.D
Acq On : 07 Oct 2022 16:00
Operator : SY/MD
Sample : N4890-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc